
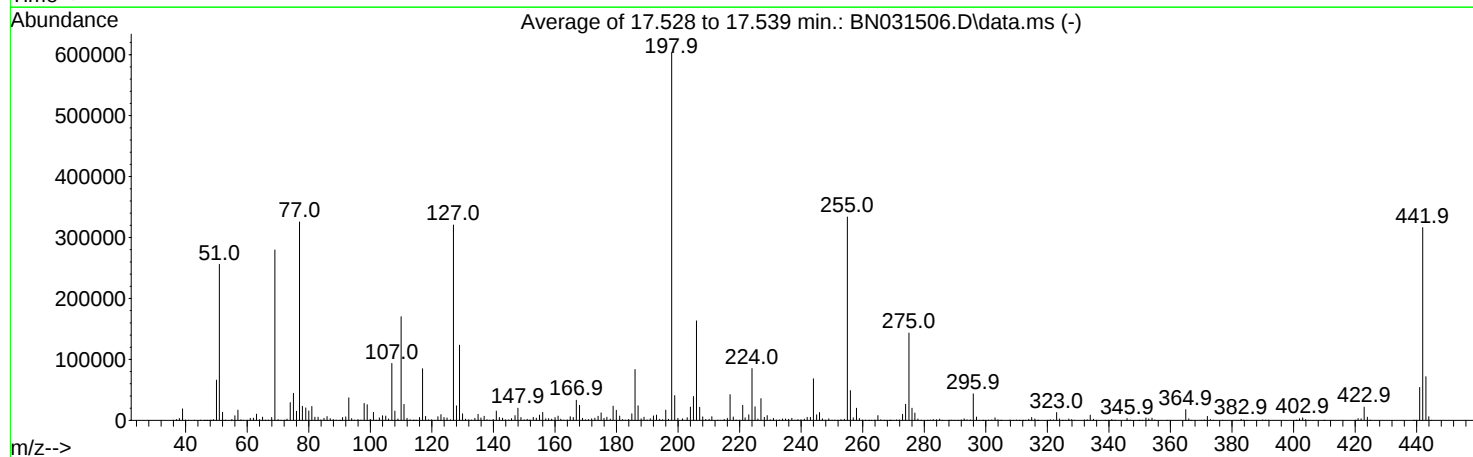


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051324\
Data File : BN031506.D
Acq On : 13 May 2024 18:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 10 02:12:24 2024

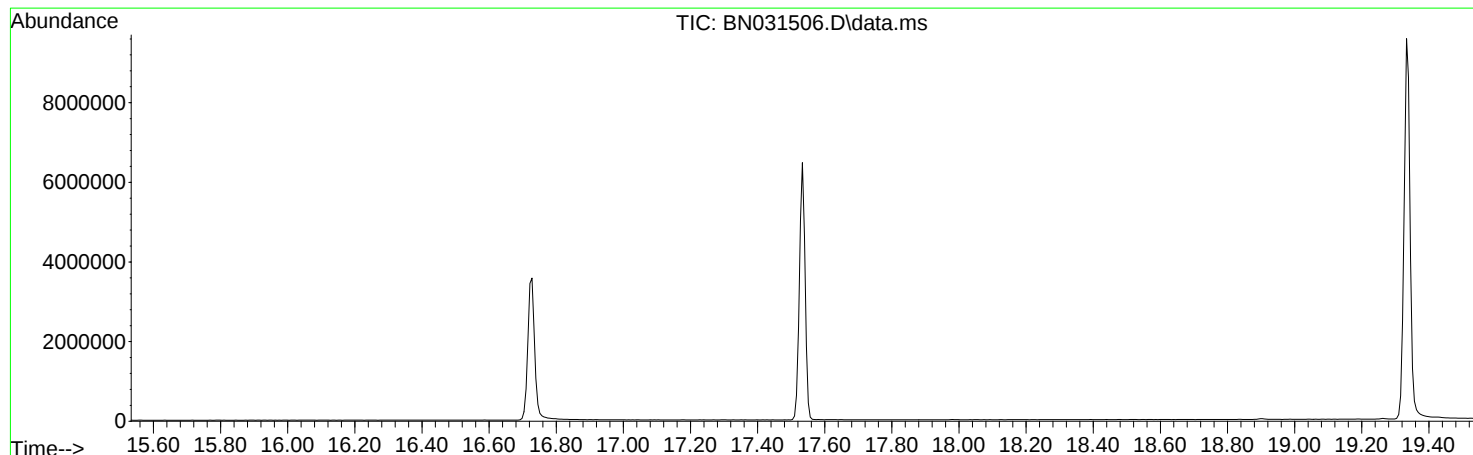

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	255858	PASS
68	69	0.00	2	1.7	4752	PASS
69	198	0.00	100	46.3	279637	PASS
70	69	0.00	2	0.5	1325	PASS
127	198	10	80	53.1	320555	PASS
197	198	0.00	2	0.3	1875	PASS
198	198	100	100	100.0	603563	PASS
199	198	5	9	6.7	40725	PASS
275	198	10	60	23.8	143408	PASS
365	198	1	100	2.9	17720	PASS
441	198	0.01	100	9.0	54064	PASS
442	442	50	100	100.0	316437	PASS
443	442	15	24	22.6	71624	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/13/2024	BNA_N	<u>BN031506.D</u>
Compound Name	Response	Retention Time
DDT	1990998	20.569
DDD	23145	20.127
DDE	923	19.622
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24068	2015066	1.19

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051324\
Data File : BN031506.D
Acq On : 13 May 2024 18:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 14 01:29:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

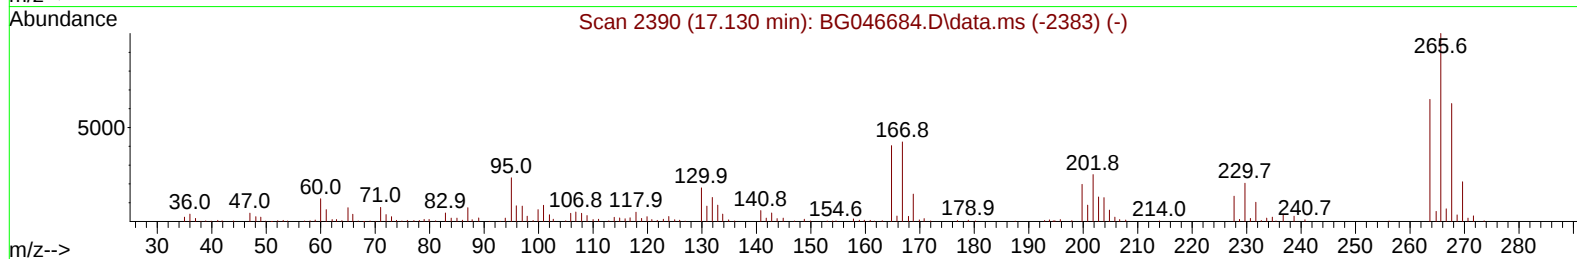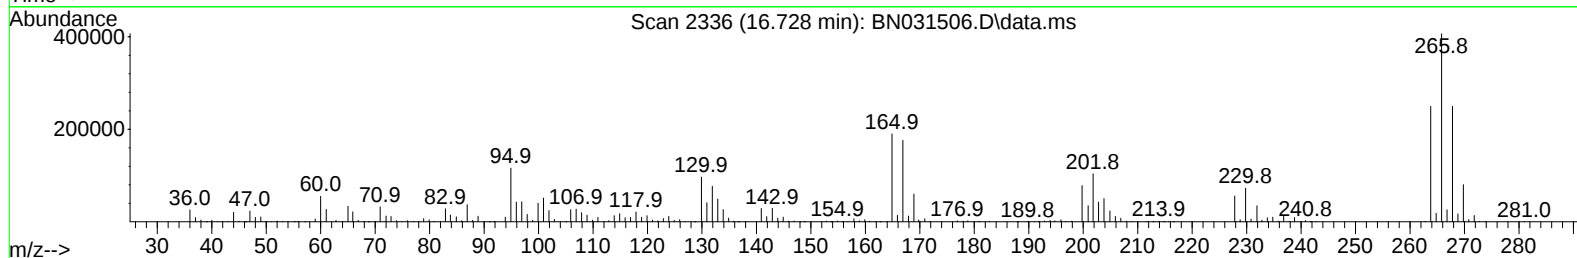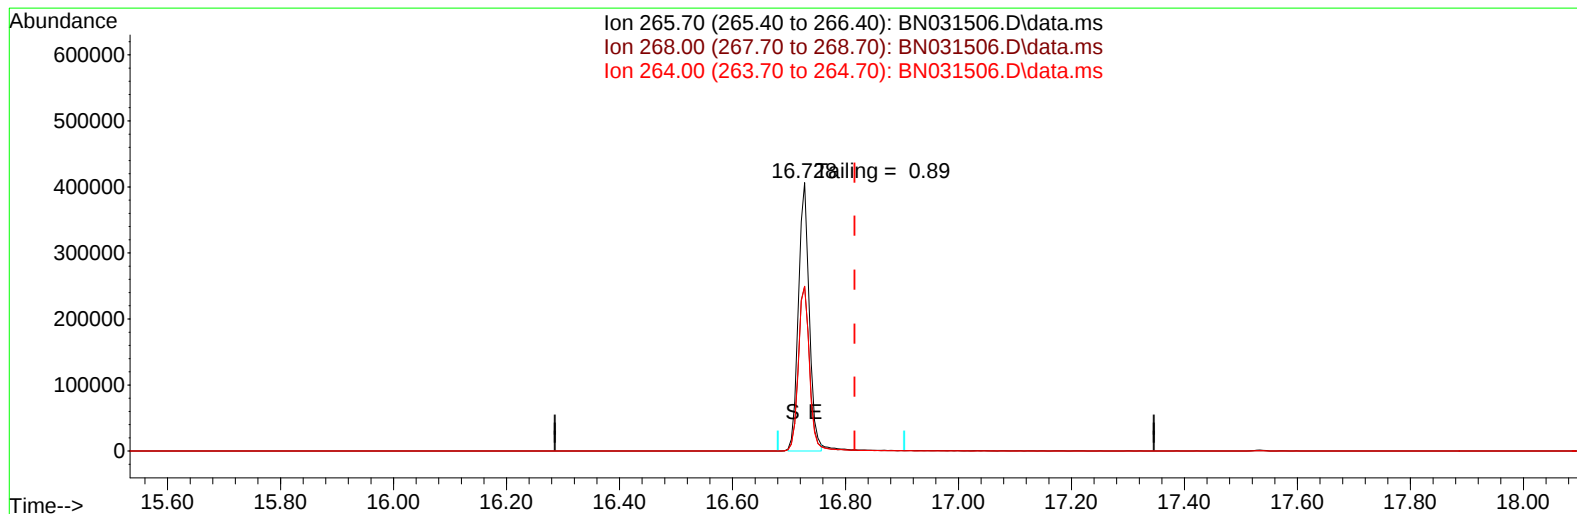

TIC: BN031506.D\data.ms

(70) Pentachlorophenol (C)

16.728min (-0.088) 19984.70 ng




response 558646

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.38
264.00	61.60	61.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051324\
Data File : BN031506.D
Acq On : 13 May 2024 18:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 14 01:29:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

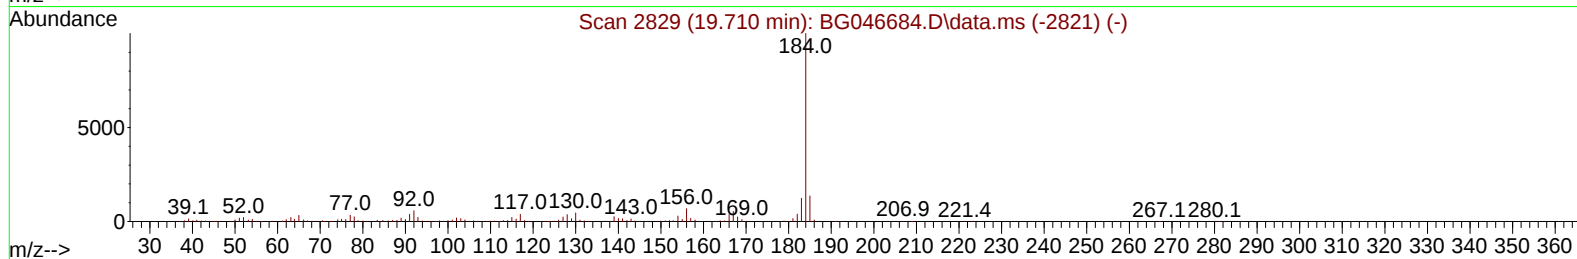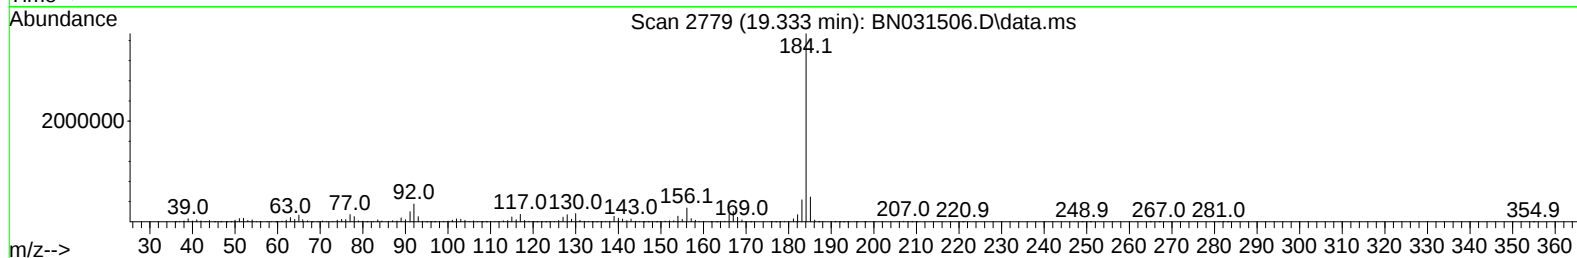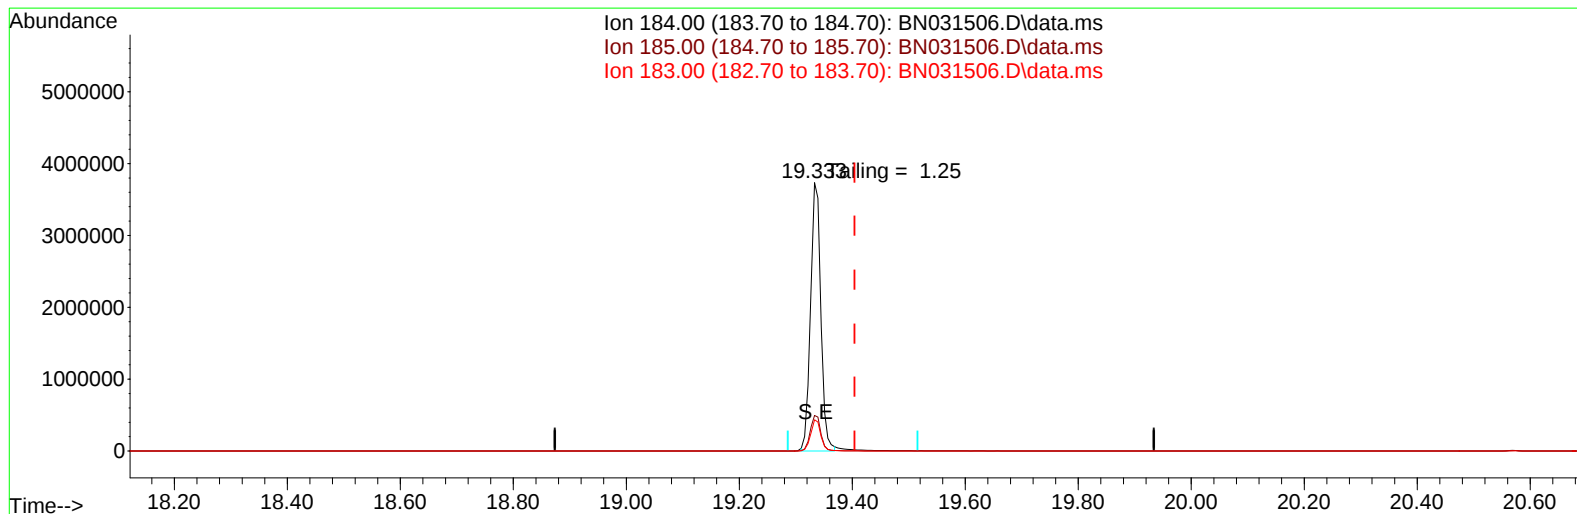

TIC: BN031506.D\data.ms

(77) Benzidine

19.333min (-0.071) 0.00 ng

response 4809267

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.24
183.00	13.20	11.67
0.00	0.00	0.00