
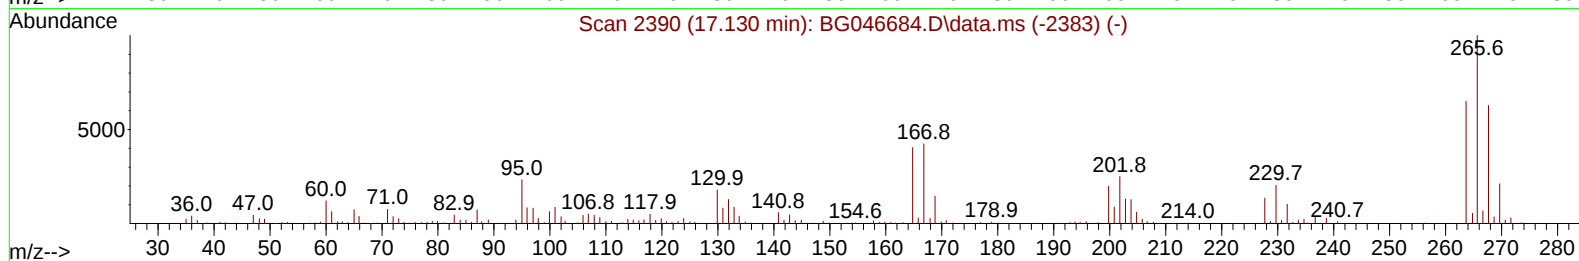
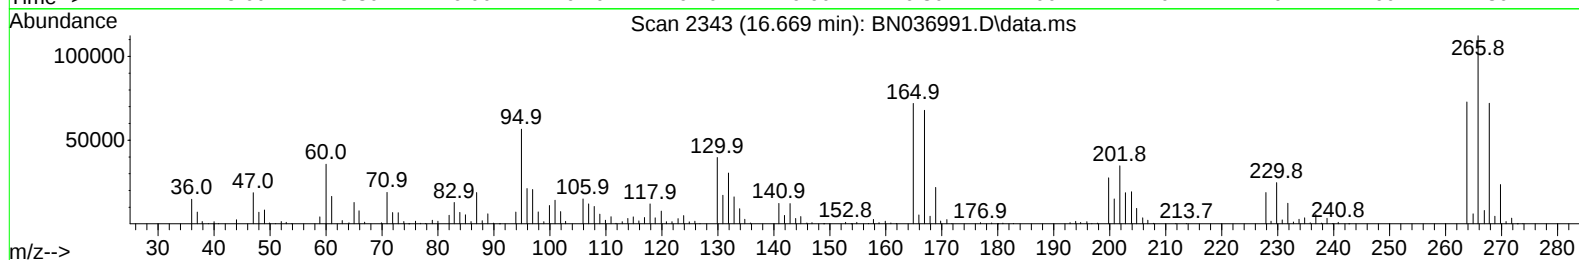


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051325\
Data File : BN036991.D
Acq On : 13 May 2025 09:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 15:42:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

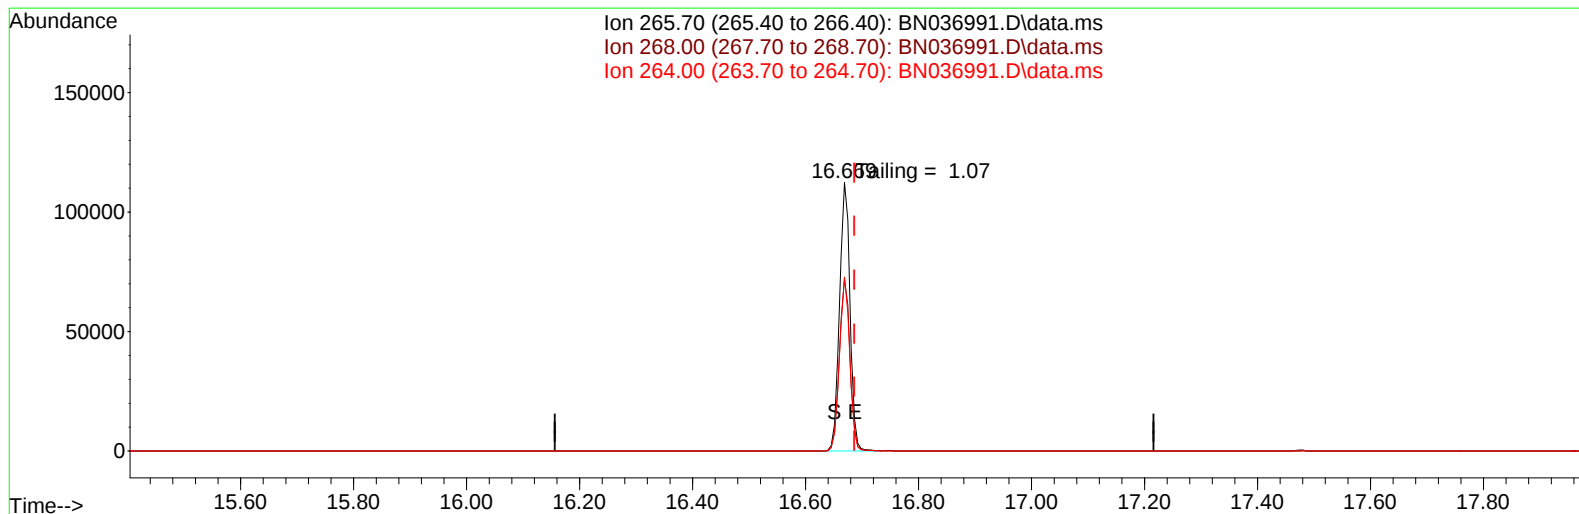

TIC: BN036991.D\data.ms

(70) Pentachlorophenol (C)




16.669min (-0.017) 16816.24 ng

response 143451

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.16
264.00	61.60	64.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051325\
Data File : BN036991.D
Acq On : 13 May 2025 09:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 15:42:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

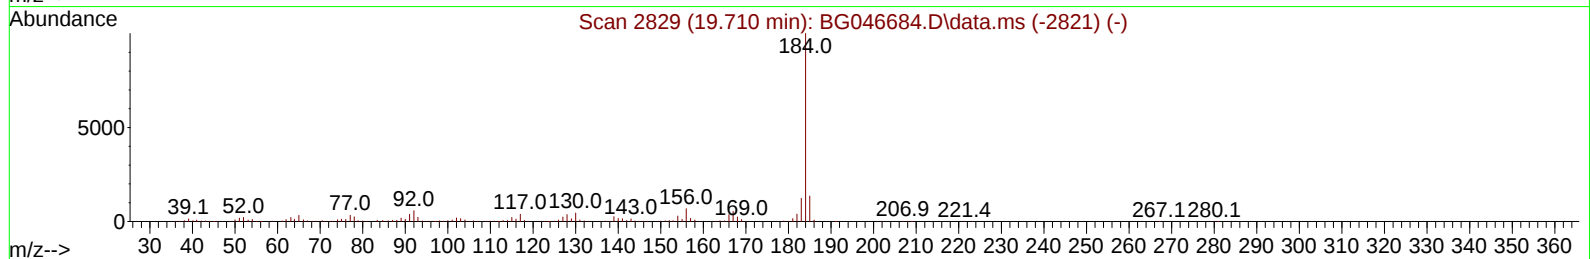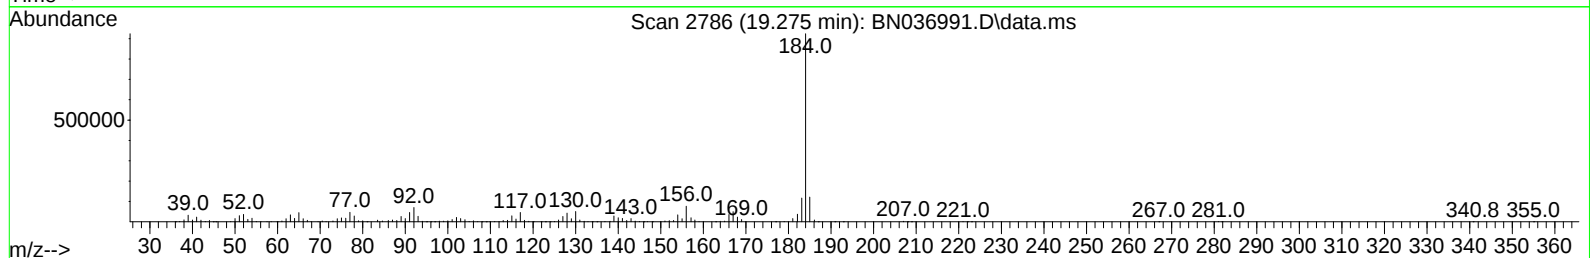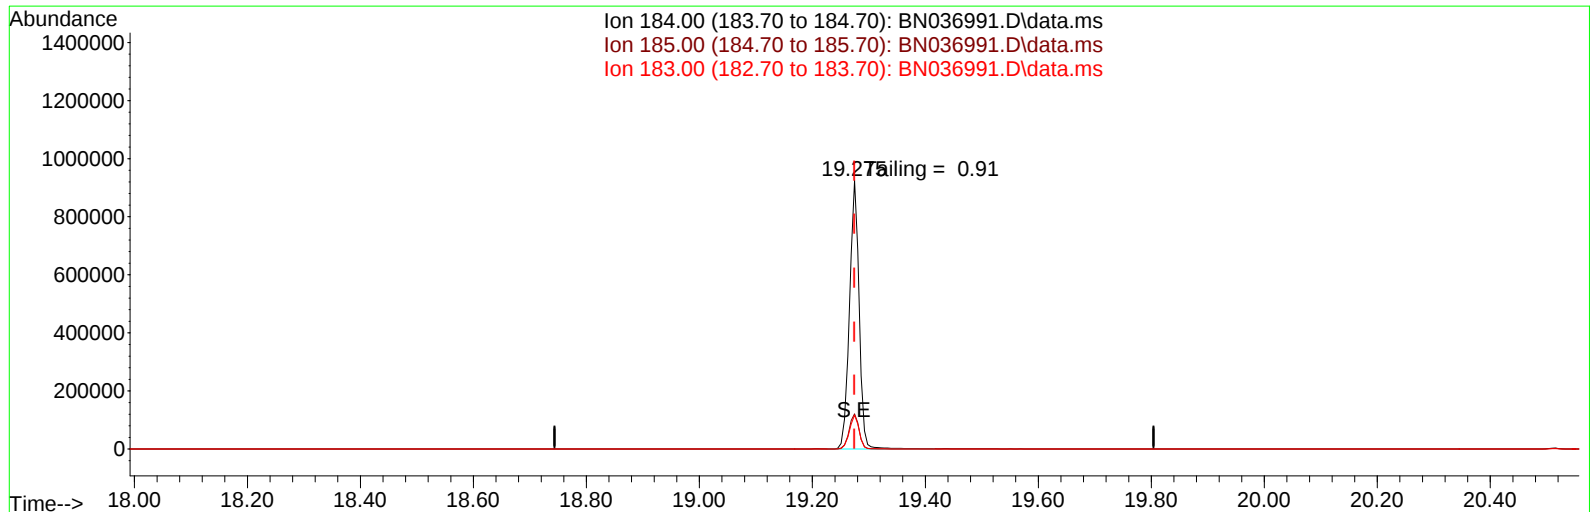

TIC: BN036991.D\data.ms

(77) Benzidine

19.275min (+ 0.000) 0.00 ng m

response 1098248

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.12
183.00	13.20	12.64
0.00	0.00	0.00