


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051420\
 Data File : BN010709.D
 Acq On : 14 May 2020 10:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 13 14:18:48 2020

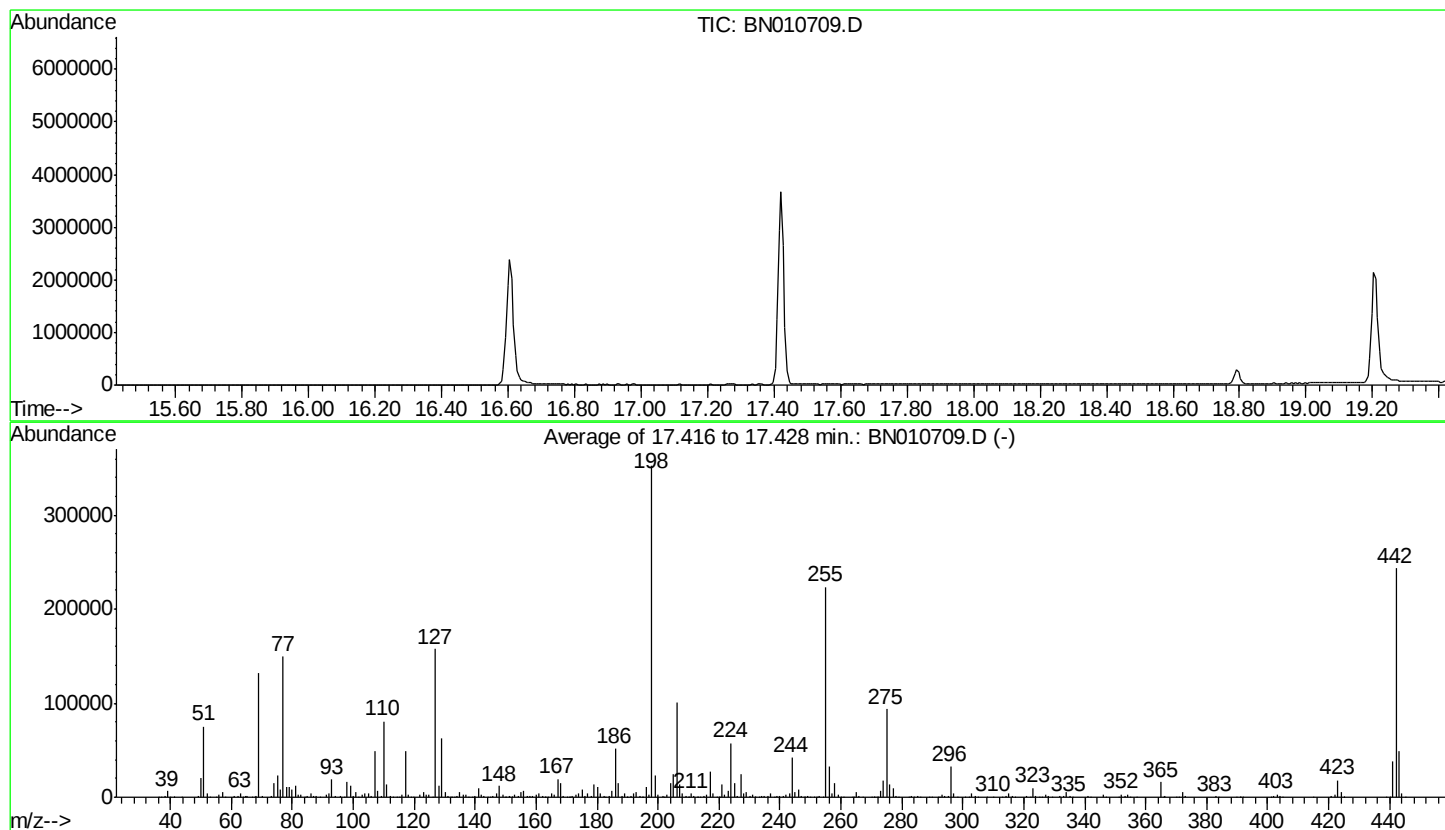

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.4	75488	PASS
68	69	0.00	2	1.5	1979	PASS
69	198	0.00	100	37.5	132066	PASS
70	69	0.00	2	0.6	763	PASS
127	198	10	80	44.8	157890	PASS
197	198	0.00	2	0.6	2182	PASS
198	198	100	100	100.0	352597	PASS
199	198	5	9	6.6	23397	PASS
275	198	10	60	26.6	93834	PASS
365	198	1	100	4.5	15801	PASS
441	198	0.01	100	10.9	38394	PASS
442	198	50	100	69.1	243562	PASS
443	442	15	24	20.2	49093	PASS