


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051421\
Data File : BN014638.D
Acq On : 14 May 2021 23:46
Operator : CG/JU
Sample : M2197-21
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YART0

Manual Integrations
APPROVED

mohammad
5/16/2021 12:16:37 AM

Quant Time: May 15 00:28:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 15:50:11 2021
Response via : Initial Calibration

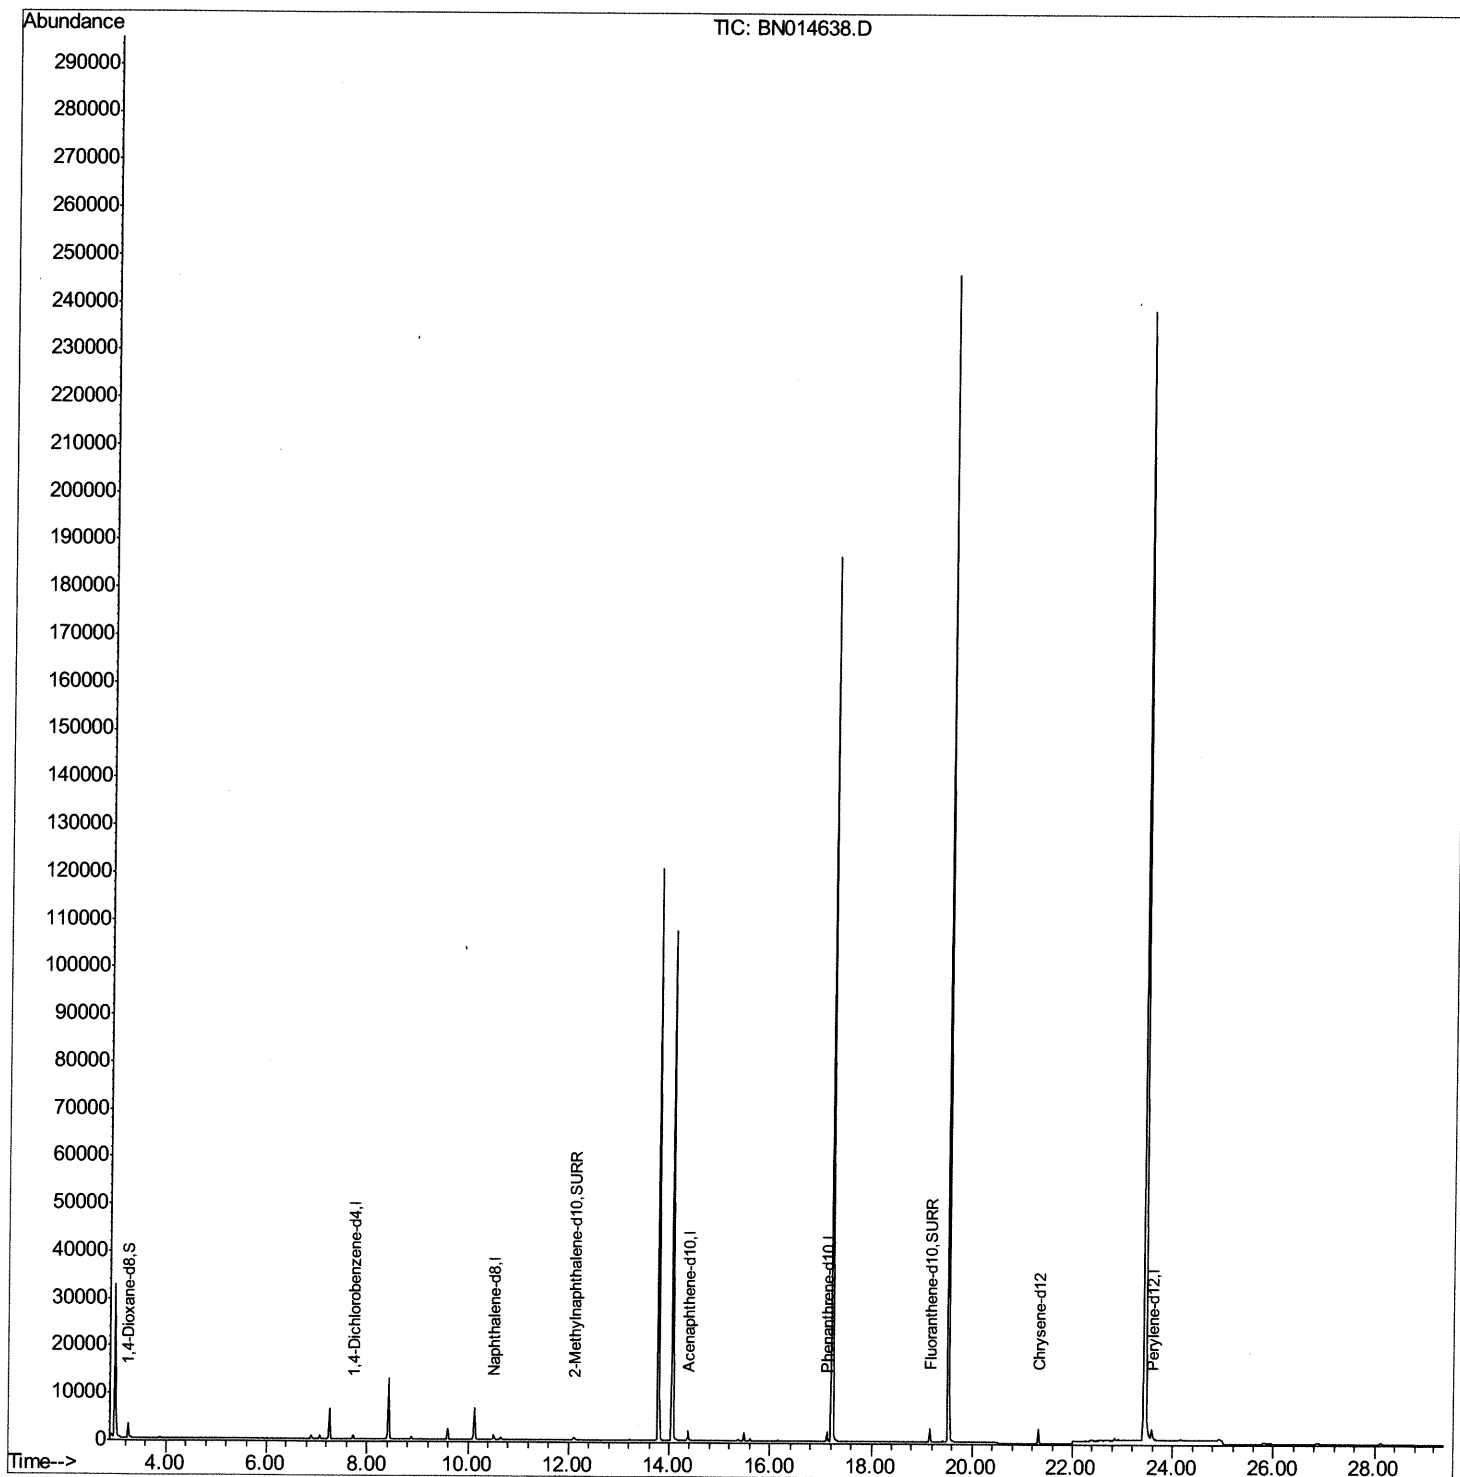

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051421\
Data File : BN014638.D
Acq On : 14 May 2021 23:46
Operator : CG/JU
Sample : M2197-21
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YART0

Manual Integrations
APPROVED

mohammad
5/16/2021 12:16:37 AM

Quant Time: May 15 00:26:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 15:50:11 2021
Response via : Initial Calibration

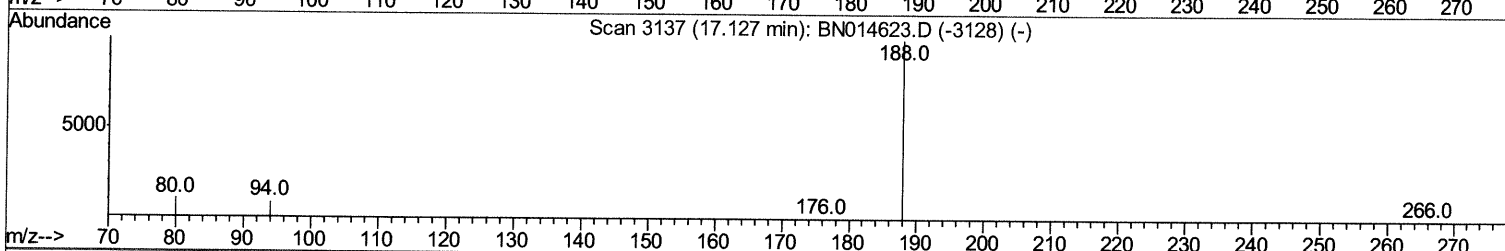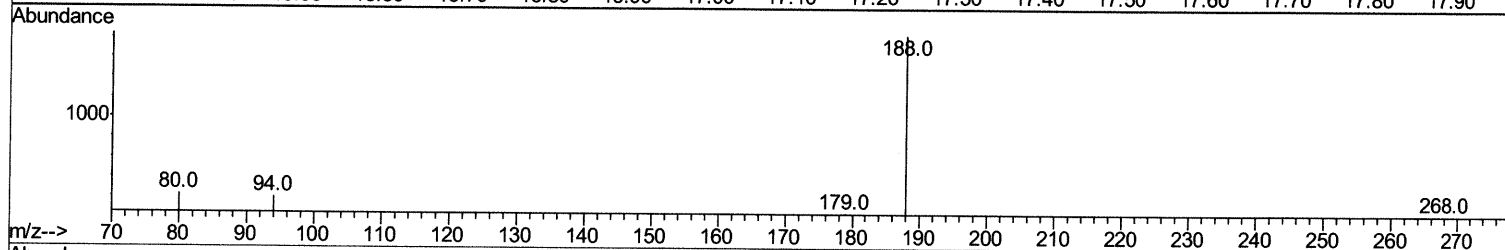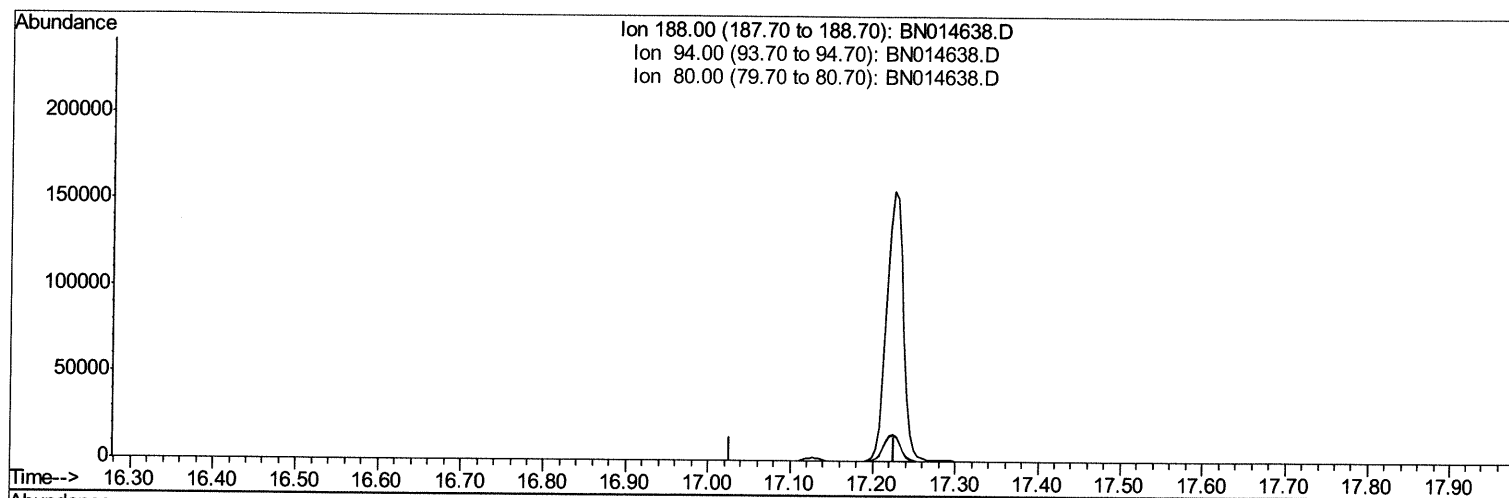

TIC: BN014638.D

(13) Phenanthrene-d10 (I)

17.127min (-17.127) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.10	0.00#
80.00	12.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051421\
Data File : BN014638.D
Acq On : 14 May 2021 23:46
Operator : CG/JU
Sample : M2197-21
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YART0

Manual Integrations
APPROVED

mohammad
5/16/2021 12:16:37 AM

Quant Time: May 15 00:26:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 15:50:11 2021
Response via : Initial Calibration

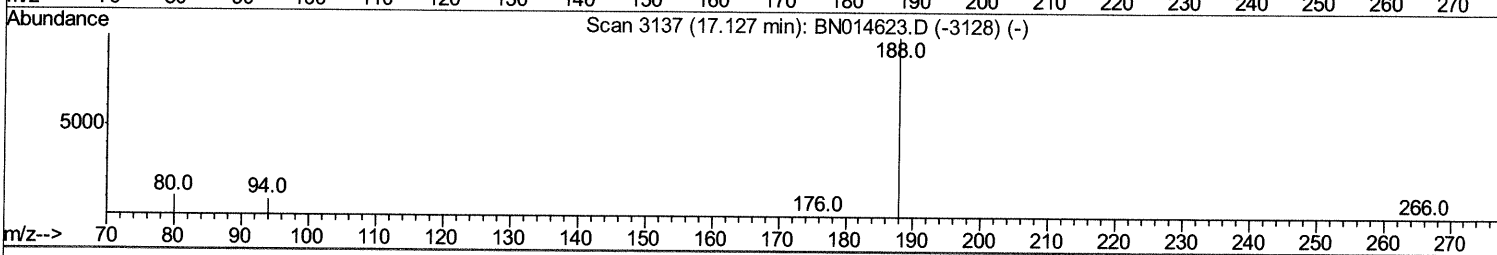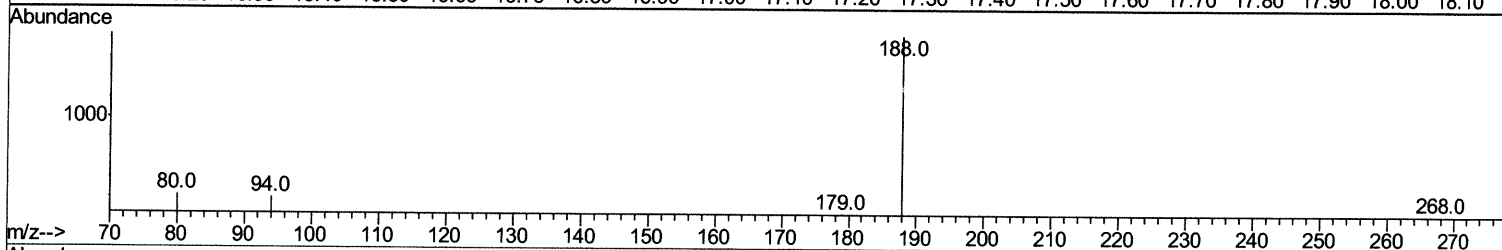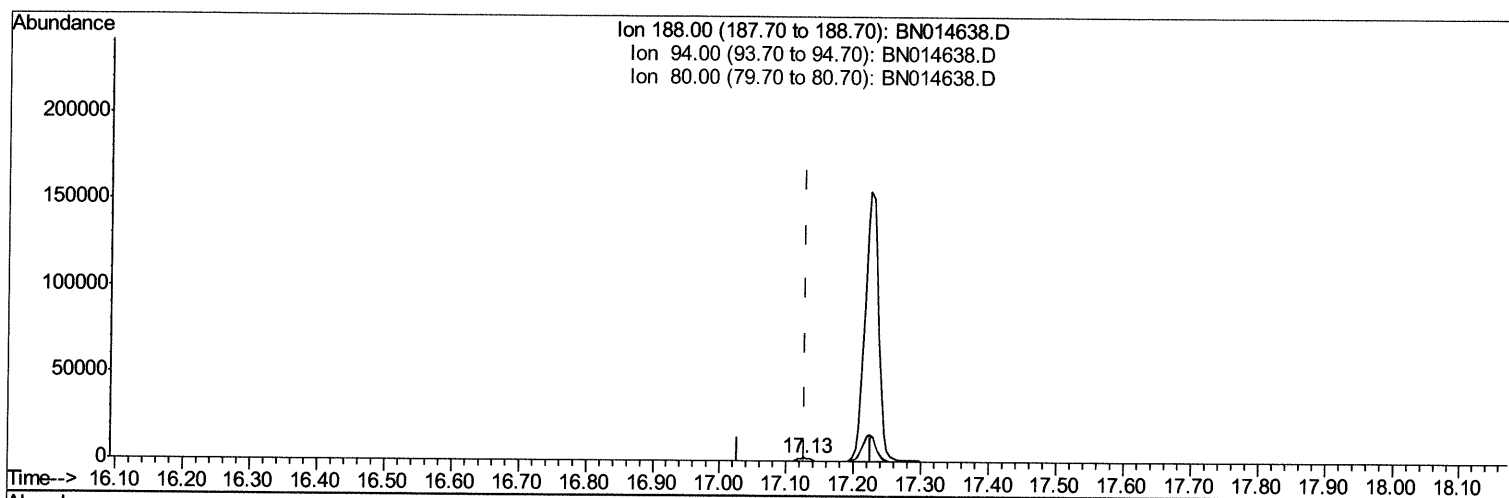

TIC: BN014638.D

(13) Phenanthrene-d10 (I)

17.127min (-0.000) 0.40ng/ul m 05/17/21 JU

response 2485

Ion	Exp%	Act%
188.00	100	100
94.00	11.10	10.85
80.00	12.50	12.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051421\
 Data File : BN014638.D
 Acq On : 14 May 2021 23:46
 Operator : CG/JU
 Sample : M2197-21
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YART0

Manual Integrations
 APPROVED

mohammad
 5/16/2021 12:16:37 AM

Quant Time: May 15 00:28:34 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 15:50:11 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	399	0.40	ng/ul	0.00
4) Naphthalene-d8	10.51	136	1327	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.38	164	1067	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.13	188	2485m>	0.40	ng/ul>	0.00051717131
17) Chrysene-d12	21.32	240	2847	0.40	ng/ul	0.00
23) Perylene-d12	23.59	264	3013	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	2320	5.67	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.11	152	799	0.35	ng/ul	0.00
18) Fluoranthene-d10	19.16	212	3195	0.44	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed