


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051421\
Data File : BN014653.D
Acq On : 15 May 2021 18:38
Operator : CG/JU
Sample : SP5563
Misc : SFAM SURROGATE80/16/0.8
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SP5563

Manual Integrations
APPROVED

mohammad
5/17/2021 11:21:00 AM

Quant Time: May 16 02:32:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 15:50:11 2021
Response via : Initial Calibration

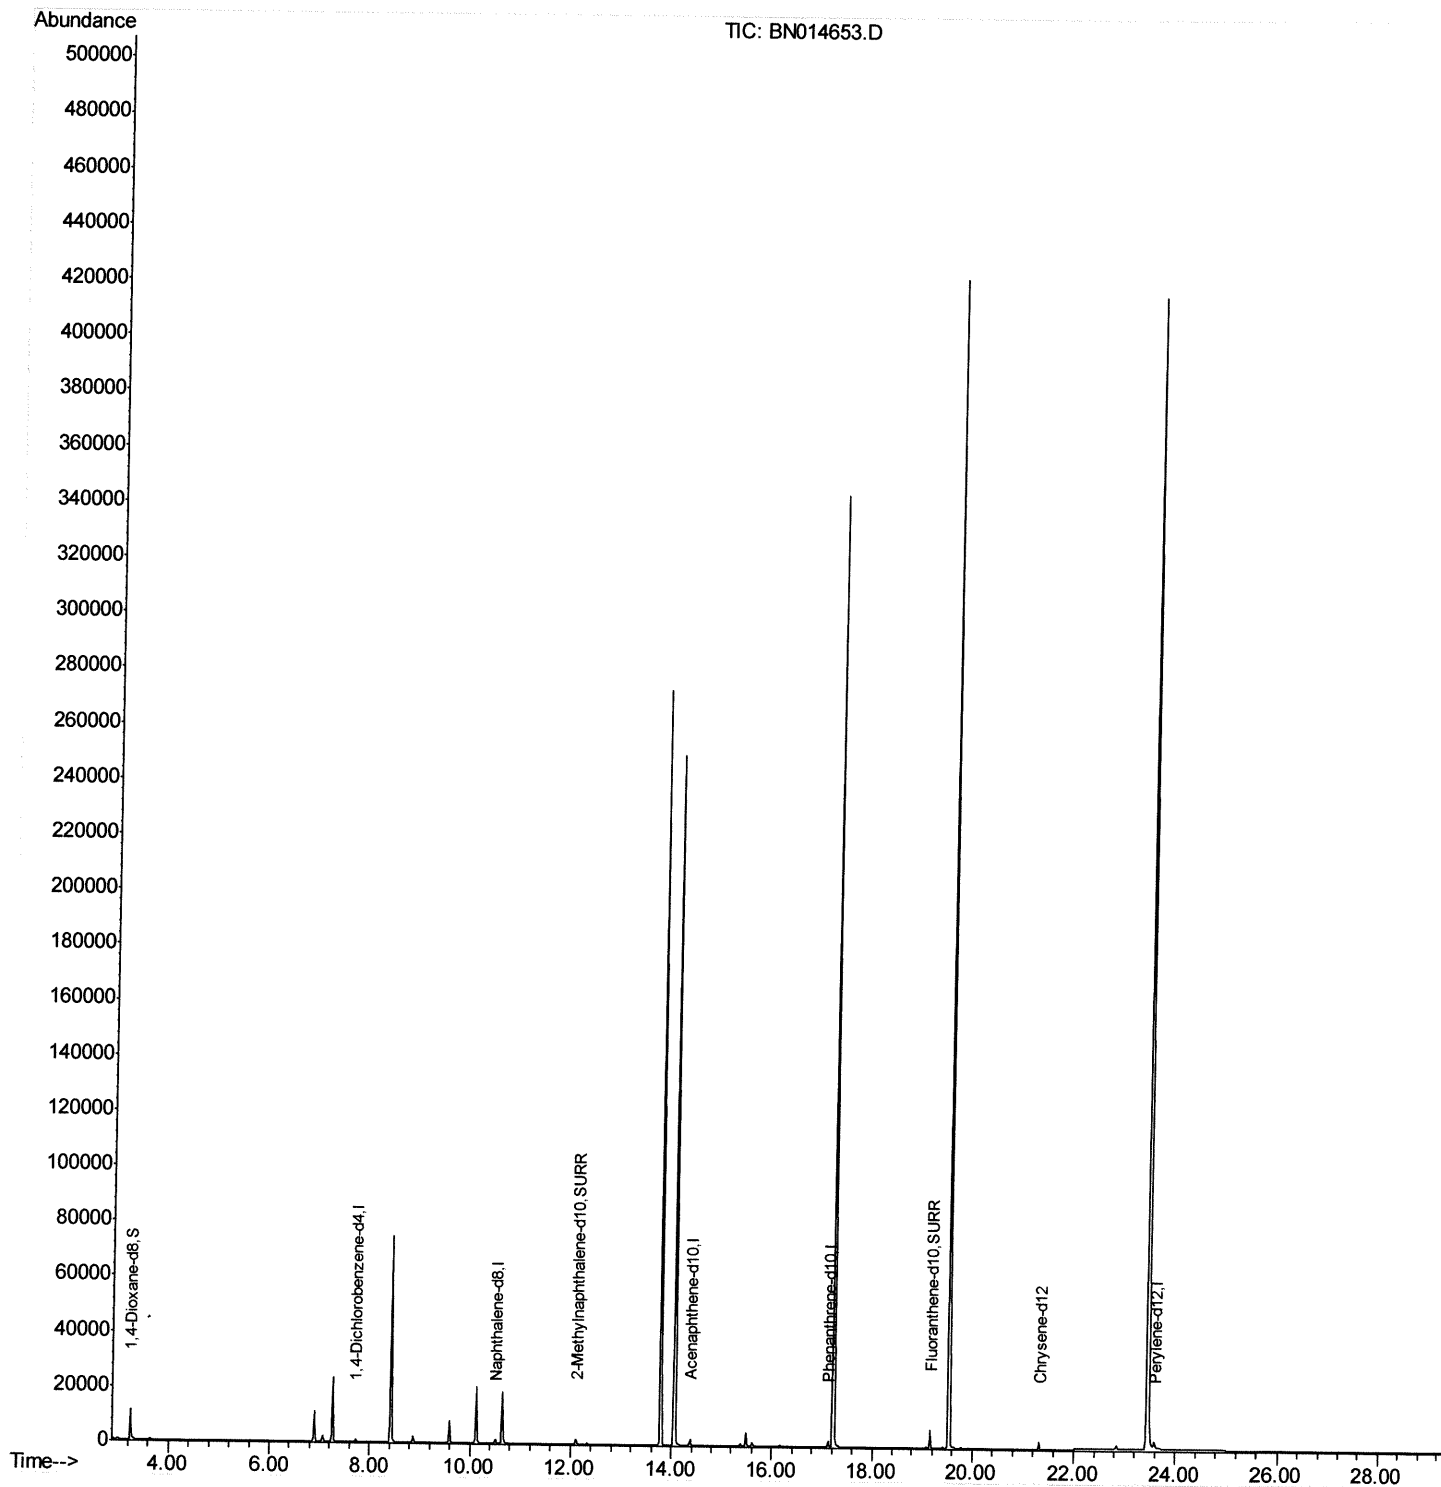

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051421\
 Data File : BN014653.D
 Acq On : 15 May 2021 18:38
 Operator : CG/JU
 Sample : SP5563
 Misc : SFAM SURROGATE80/16/0.8
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 SP5563

Manual Integrations
APPROVED

mohammad
 5/17/2021 11:21:00 AM

Quant Time: May 16 02:00:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 15:50:11 2021
 Response via : Initial Calibration

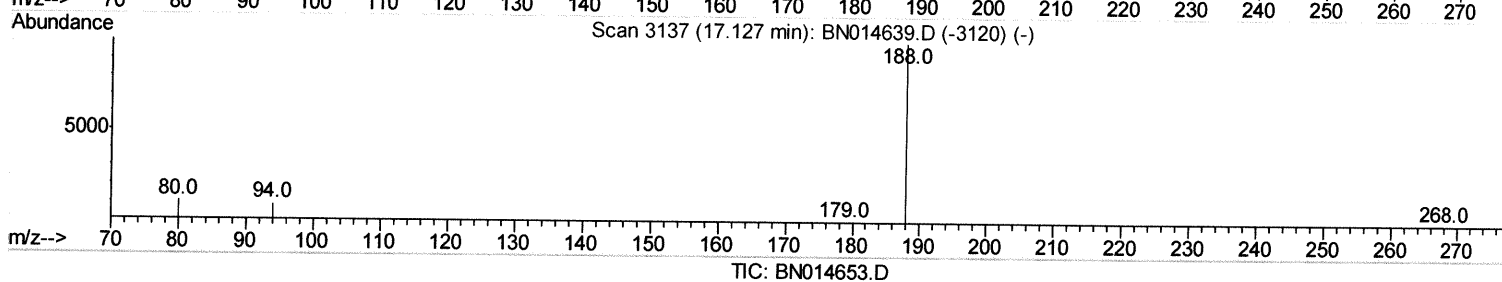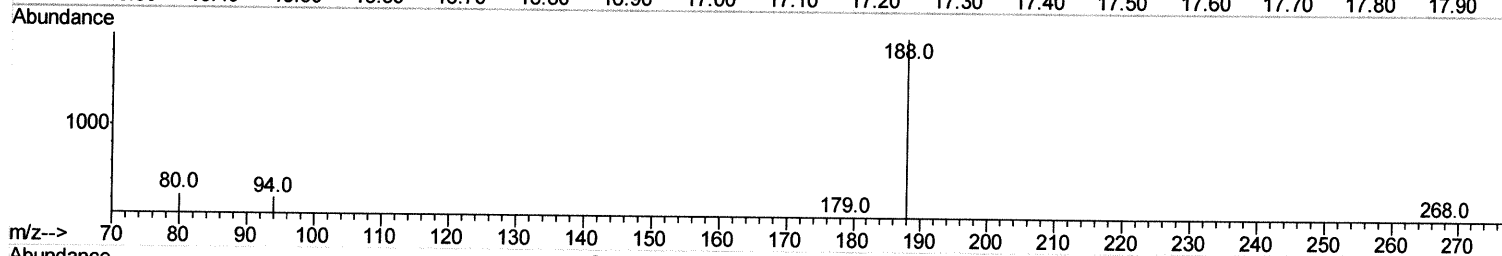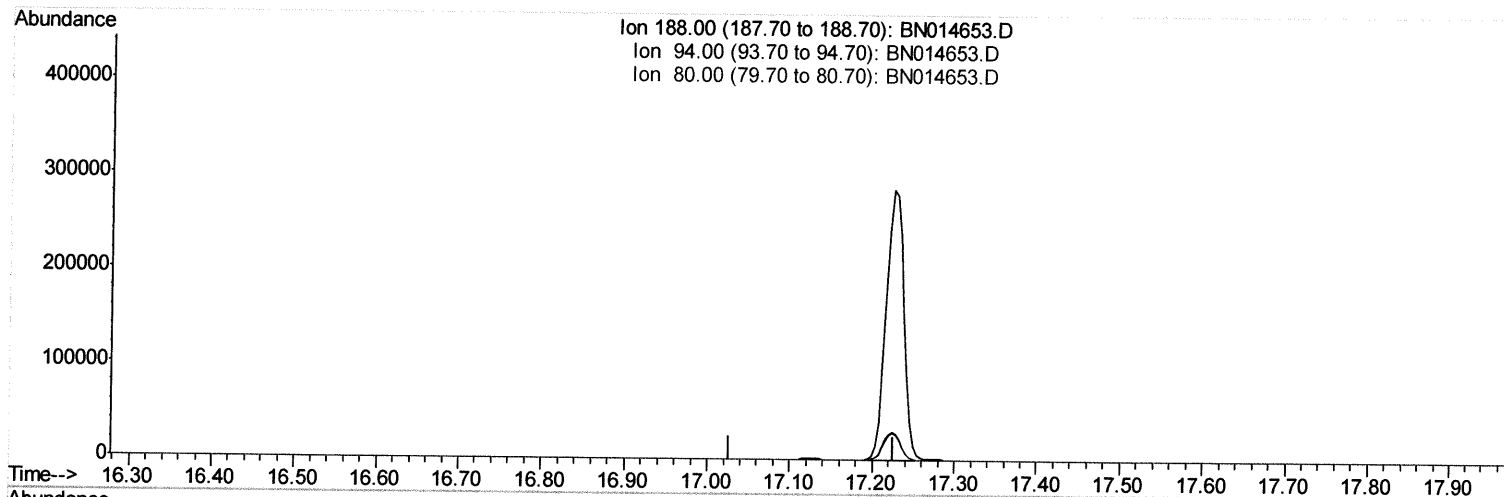

(13) Phenanthrene-d10 (I)

17.127min (-17.127) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.10	0.00#
80.00	12.50	0.00#
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051421\
Data File : BN014653.D
Acq On : 15 May 2021 18:38
Operator : CG/JU
Sample : SP5563
Misc : SFAM SURROGATE80/16/0.8
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SP5563

Manual Integrations
APPROVED

mohammad
5/17/2021 11:21:00 AM

Quant Time: May 16 02:00:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 15:50:11 2021
Response via : Initial Calibration

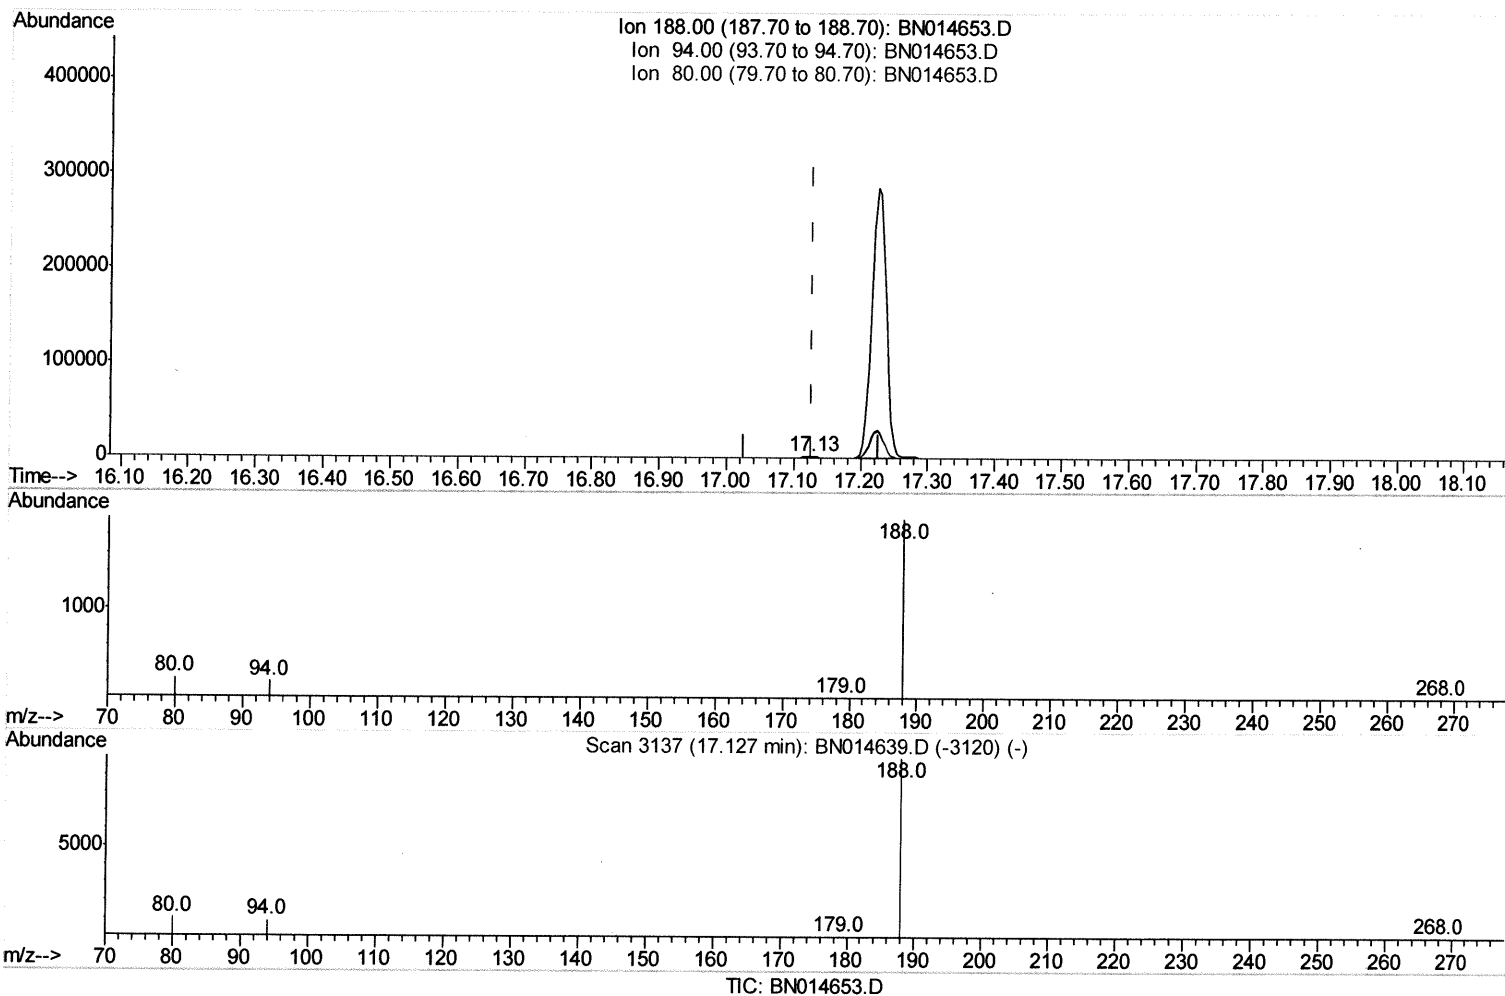

(13) Phenanthrene-d10 (I)

17.127min (+0.000) 0.40ng/ul m JU 5/17/21

response 2670

Ion	Exp%	Act%
188.00	100	100
94.00	11.10	10.93
80.00	12.50	12.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051421\
 Data File : BN014653.D
 Acq On : 15 May 2021 18:38
 Operator : CG/JU
 Sample : SP5563
 Misc : SFAM SURROGATE80/16/0.8
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SP5563

Manual Integrations
 APPROVED

mohammad
 5/17/2021 11:21:00 AM

Quant Time: May 16 02:32:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 15:50:11 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	433	0.40	ng/ul	0.00
4) Naphthalene-d8	10.51	136	1481	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.38	164	1257	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.13	188	2670m	0.40	ng/ul	0.00
17) Chrysene-d12	21.32	240	2703	0.40	ng/ul	0.00
23) Perylene-d12	23.58	264	2967	0.40	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	8243	18.56	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.11	152	2484	0.97	ng/ul	0.00
18) Fluoranthene-d10	19.16	212	7439	1.09	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed