

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN051421\
 Data File : BN014632.D
 Acq On : 14 May 2021 19:38
 Operator : CG/JU
 Sample : PB136090BS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLCS090

Quant Time: May 14 23:29:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 15:50:11 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	434	0.40	ng/ul	0.00
4) Naphthalene-d8	10.52	136	1358	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.38	164	951	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.13	188	2413	0.40	ng/ul	0.00
17) Chrysene-d12	21.32	240	3013	0.40	ng/ul	0.00
23) Perylene-d12	23.59	264	2494	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	268	0.60	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.11	152	767	0.33	ng/ul	0.00
18) Fluoranthene-d10	19.16	212	2730	0.36	ng/ul	0.00
Target Compounds				Ovalue		
2) 1,4-Dioxane	3.28	88	727	1.562	ng/ul#	85
5) Naphthalene	10.57	128	1270	0.322	ng/ul	98
7) 2-Methylnaphthalene	12.18	142	894	0.315	ng/ul	98
8) 1-Methylnaphthalene	12.40	142	877	0.320	ng/ul	98
10) Acenaphthylene	14.09	152	1050	0.305	ng/ul	100
11) Acenaphthene	14.44	153	1025	0.313	ng/ul	99
12) Fluorene	15.43	166	1268	0.315	ng/ul	96
14) Pentachlorophenol	16.78	266	213	0.627	ng/ul	92
15) Phenanthrene	17.17	178	2453	0.327	ng/ul	98
16) Anthracene	17.26	178	1931	0.330	ng/ul	98
19) Fluoranthene	19.19	202	3271	0.349	ng/ul	96
20) Pyrene	19.55	202	3272	0.345	ng/ul	98
21) Benzo(a)anthracene	21.31	228	3451	0.363	ng/ul	98
22) Chrysene	21.36	228	4075	0.374	ng/ul	99
24) Benzo(b)fluoranthene	22.90	252	3867	0.353	ng/ul	98
25) Benzo(k)fluoranthene	22.95	252	4149	0.359	ng/ul	98
26) Benzo(a)pyrene	23.49	252	3082	0.368	ng/ul	94
27) Indeno(1,2,3-cd)pyrene	25.88	276	4473	0.375	ng/ul#	100
28) Dibenzo(a,h)anthracene	25.89	278	3606	0.377	ng/ul	98
29) Benzo(g,h,i)perylene	26.58	276	3747	0.368	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN051421\
Data File : BN014632.D
Acq On : 14 May 2021 19:38
Operator : CG/JU
Sample : PB136090BS
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLCS090

Quant Time: May 14 23:29:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 15:50:11 2021
Response via : Initial Calibration

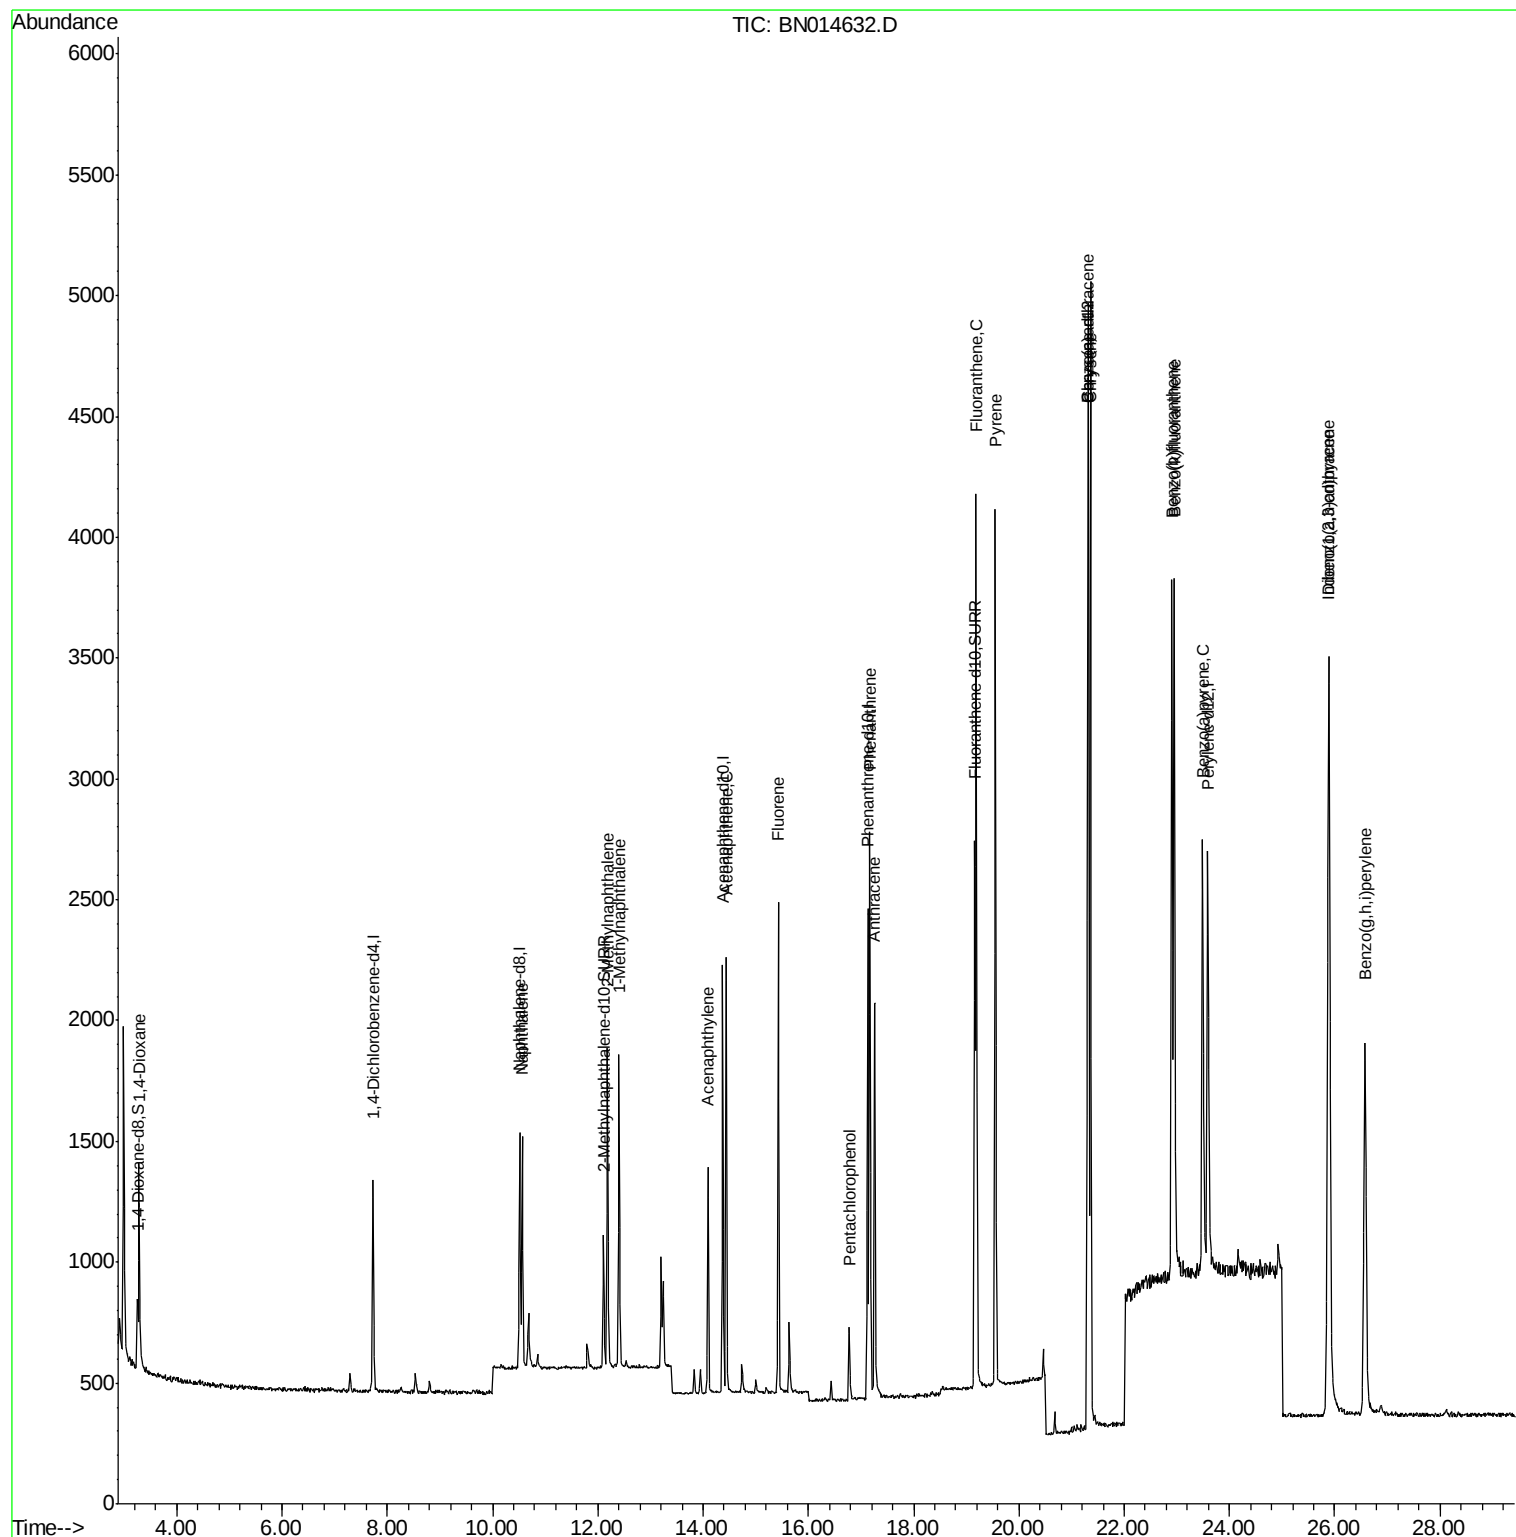

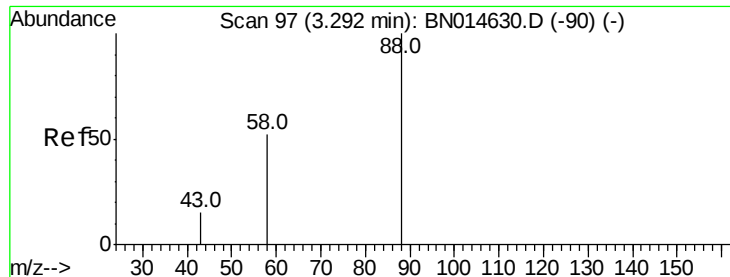

#2

1,4-Dioxane

Concen: 1.562 ng/ul

RT: 3.28 min Scan# 95

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38

Instrument :

BNA_N

ClientSampleId :

SLCS090


Tot Ion: 88 Resp: 727

Ion Ratio Lower Upper

88 100

43 21.5 22.5 33.7#




58 47.7 30.4 45.6#

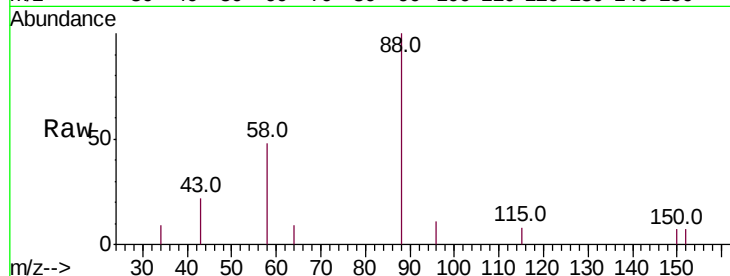

Abundance Ion 88.00 (87.70 to 88.70): BN0

Ion 43.00 (42.70 to 43.70): BN0

Ion 58.00 (57.70 to 58.70): BN0

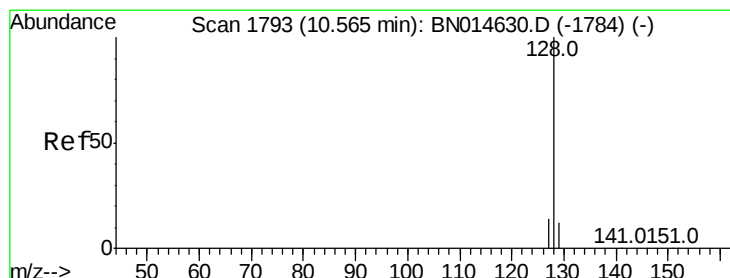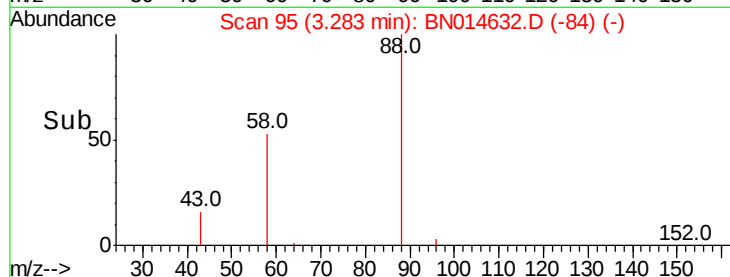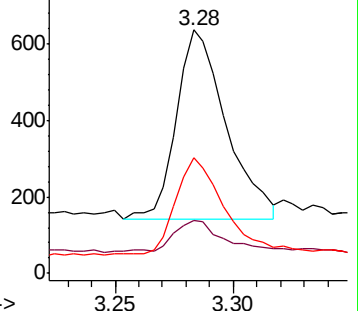

#5

Naphthalene

Concen: 0.322 ng/ul

RT: 10.57 min Scan# 1793

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38


Tgt Ion: 128 Resp: 1270

Ion Ratio Lower Upper

128 100

129 15.7 10.9 16.3



127 19.5 15.7 23.5

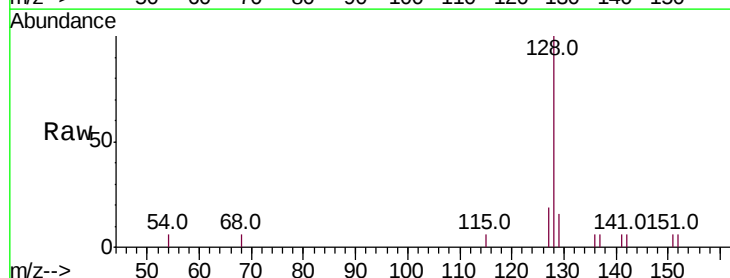


Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

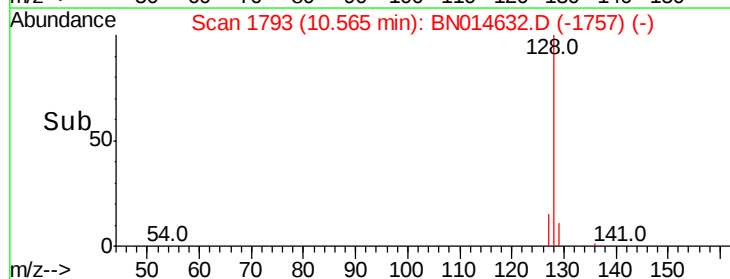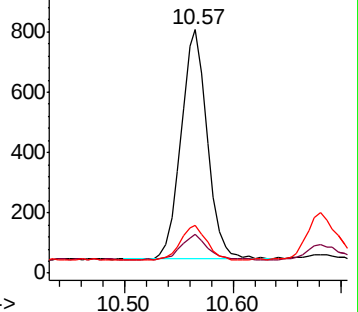

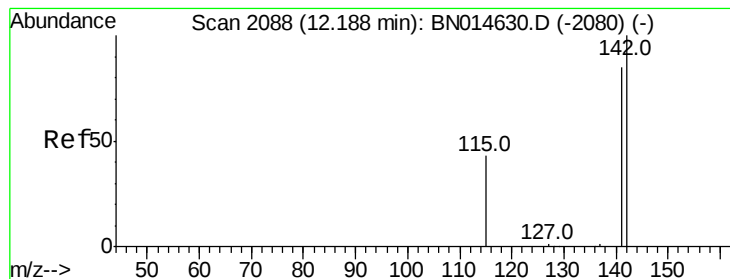

#7

2-Methylnaphthalene

Concen: 0.315 ng/ul

RT: 12.18 min Scan# 2087

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38

Instrument :

BNA_N

ClientSampleId :


SLCS090

Tot Ion:142 Resp: 894

Ion Ratio Lower Upper




142 100

141 89.3 70.2 105.2

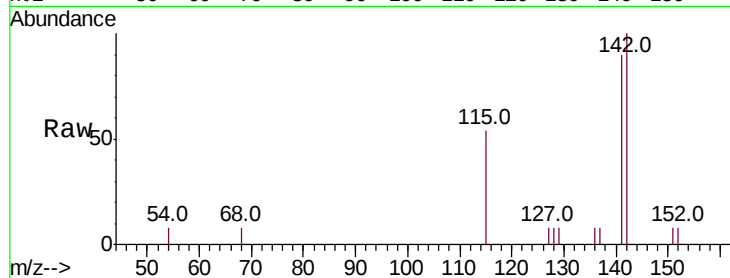

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

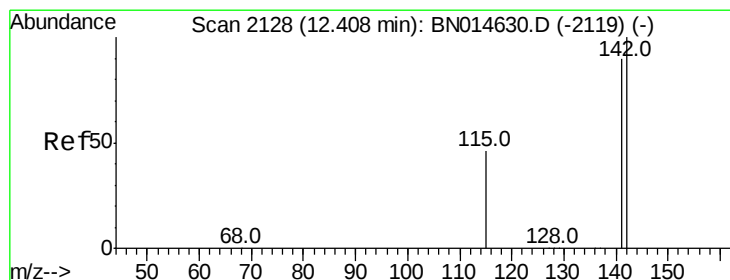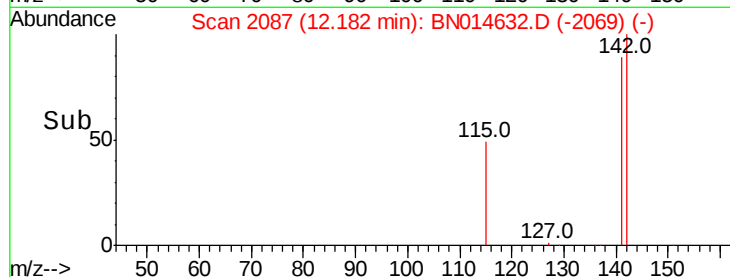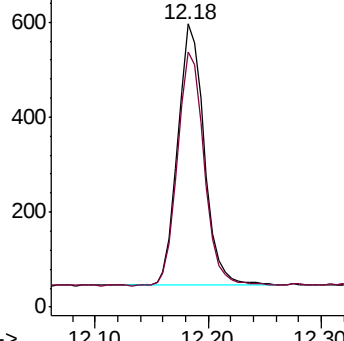

#8

1-Methylnaphthalene

Concen: 0.320 ng/ul

RT: 12.40 min Scan# 2127

Delta R.T. -0.00 min

Lab File: BN014632.D


Acq: 14 May 2021 19:38

Tgt Ion:142 Resp: 877

Ion Ratio Lower Upper



142 100


141 90.8 73.9 110.9

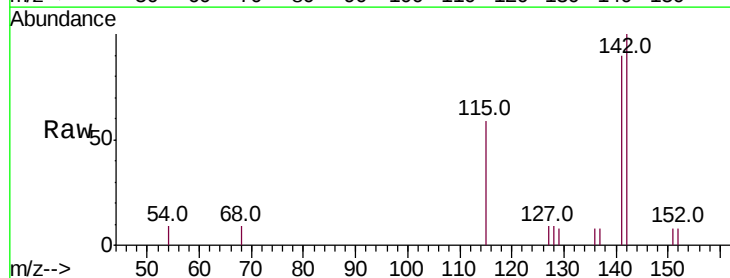

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

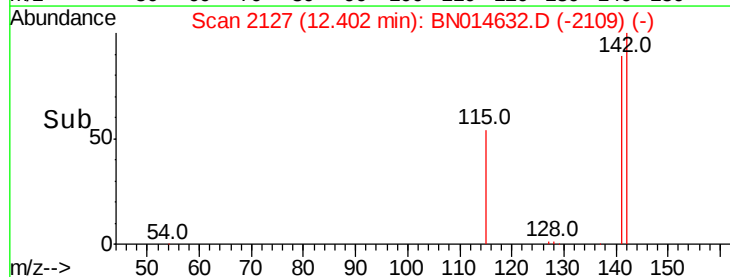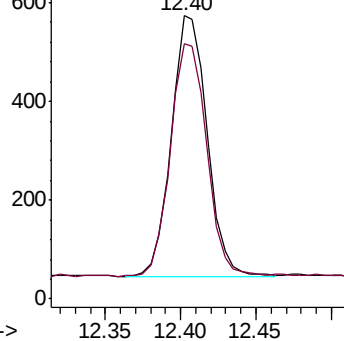



#10

Acenaphthylene

Concen: 0.305 ng/ul

RT: 14.09 min Scan# 2458

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38

Instrument :

BNA_N

ClientSampleId :

SLCS090


Tot Ion:152 Resp: 1050

Ion Ratio Lower Upper

152 100

151 25.4 20.2 30.4




153 17.4 14.2 21.4



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

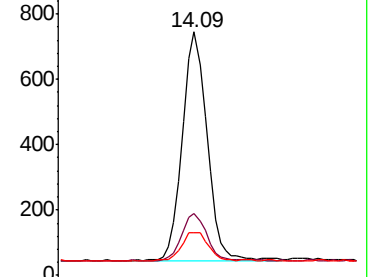

#11

Acenaphthene

Concen: 0.313 ng/ul

RT: 14.44 min Scan# 2533

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38


Tgt Ion:153 Resp: 1025

Ion Ratio Lower Upper

153 100

152 51.3 39.7 59.5



154 88.2 71.0 106.4




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

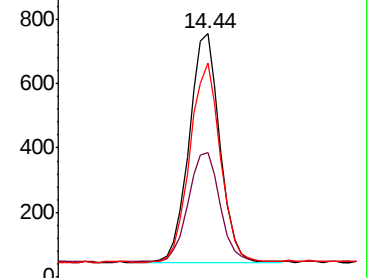

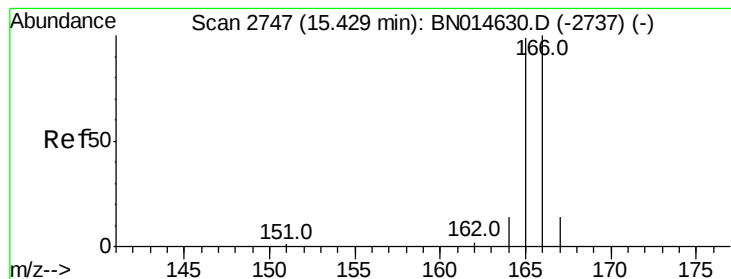

#12

Fluorene

Concen: 0.315 ng/ul

RT: 15.43 min Scan# 2747

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38

Instrument :

BNA_N

ClientSampleId :

SLCS090


Tot Ion:166 Resp: 1268

Ion Ratio Lower Upper

166 100

165 103.4 79.3 118.9




167 17.5 13.8 20.6



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

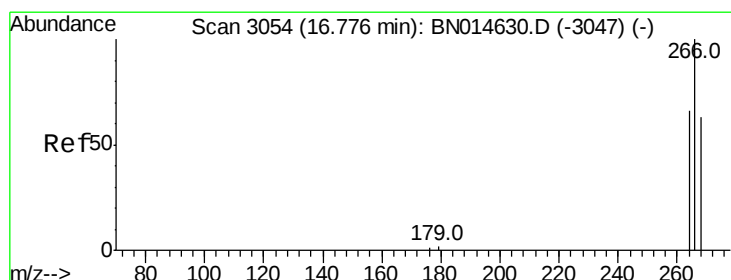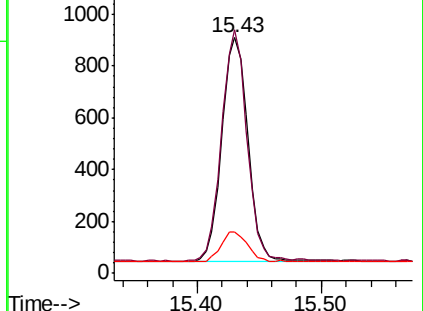

#14

Pentachlorophenol

Concen: 0.627 ng/ul

RT: 16.78 min Scan# 3055

Delta R.T. 0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38


Tgt Ion:266 Resp: 213

Ion Ratio Lower Upper

266 100

264 62.4 52.9 79.3



268 64.8 59.4 89.0




Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

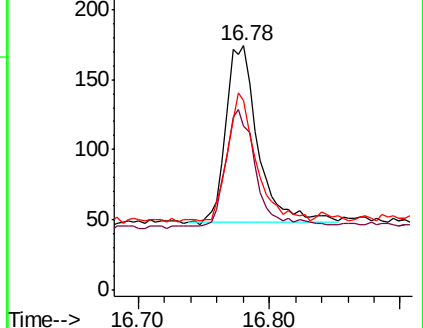



#15

Phenanthrene

Concen: 0.327 ng/ul

RT: 17.17 min Scan# 3147

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38

Instrument :

BNA_N

ClientSampleId :

SLCS090





Tot Ion:178 Resp: 2453

Ion Ratio Lower Upper

178 100

179 18.2 13.8 20.6

176 21.3 16.2 24.4

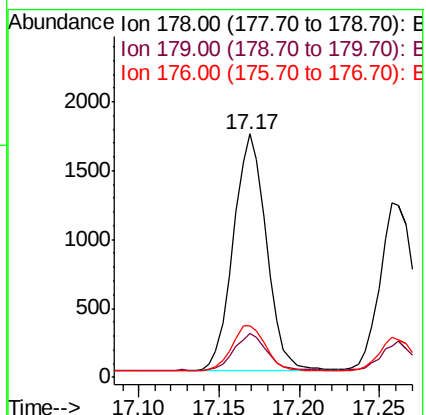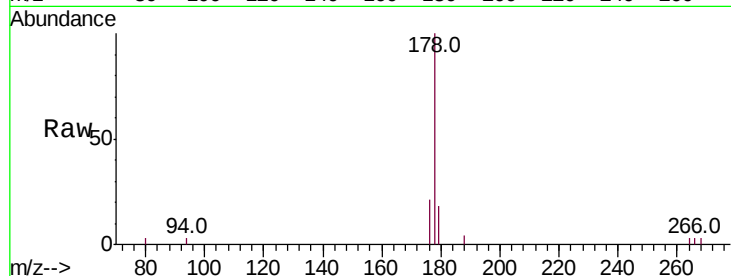

#16

Anthracene

Concen: 0.330 ng/ul

RT: 17.26 min Scan# 3168

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38




Tgt Ion:178 Resp: 1931


Ion Ratio Lower Upper

178 100

179 17.9 14.3 21.5

176 22.8 17.1 25.7

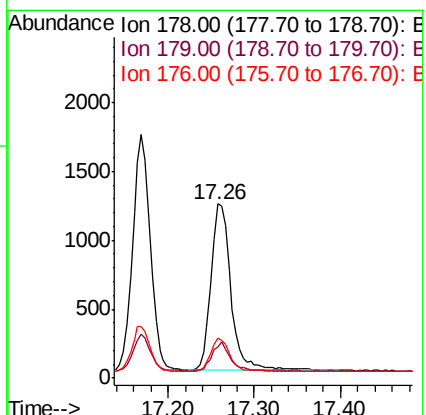



#19

Fluoranthene

Concen: 0.349 ng/ul

RT: 19.19 min Scan# 3611

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38

Instrument :

BNA_N

ClientSampleId :

SLCS090


Tot Ion:202 Resp: 3271

Ion Ratio Lower Upper

202 100

101 10.7 7.6 11.4




100 8.8 5.9 8.9

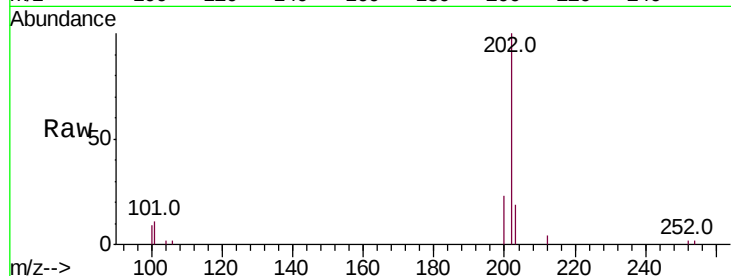

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

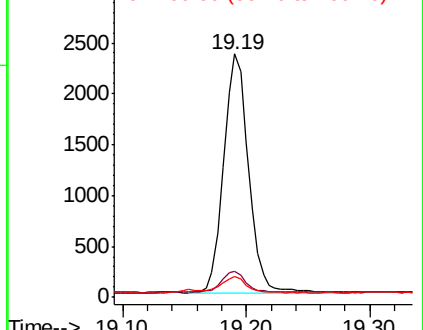

#20

Pyrene

Concen: 0.345 ng/ul

RT: 19.55 min Scan# 3689

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38


Tgt Ion:202 Resp: 3272

Ion Ratio Lower Upper

202 100

101 12.0 8.5 12.7



100 9.2 7.4 11.2




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

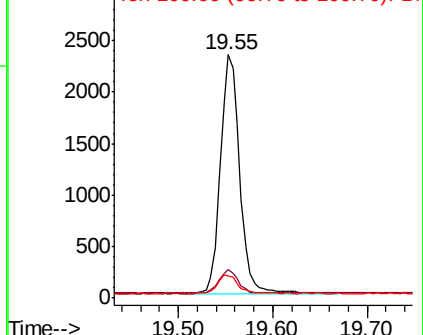

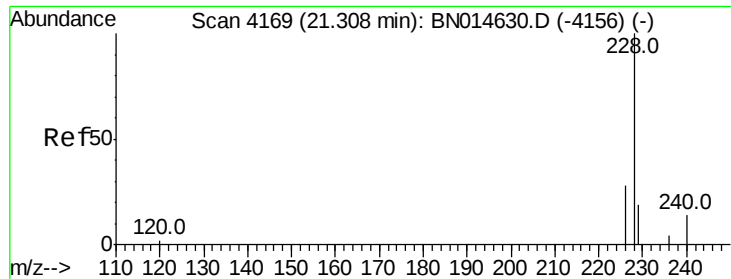

#21

Benzo(a)anthracene

Concen: 0.363 ng/ul

RT: 21.31 min Scan# 4168

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38

Instrument :

BNA_N

ClientSampleId :

SLCS090


Tot Ion:228 Resp: 3451

Ion Ratio Lower Upper




228 100

229 19.5 16.3 24.5

226 29.2 22.6 33.8

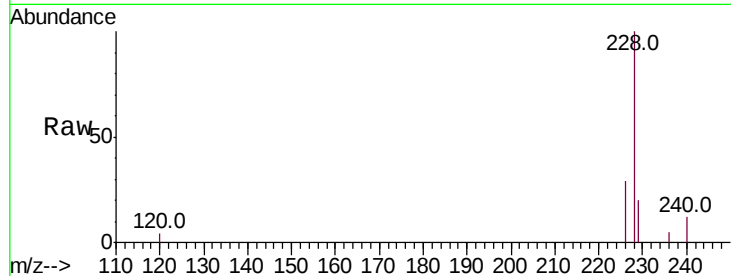

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

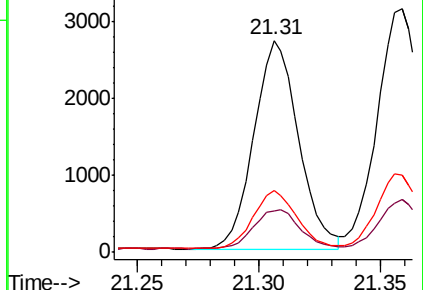

#22

Chrysene

Concen: 0.374 ng/ul

RT: 21.36 min Scan# 4186

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38


Tgt Ion:228 Resp: 4075

Ion Ratio Lower Upper



228 100


226 31.7 25.3 37.9

229 21.6 16.2 24.4



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

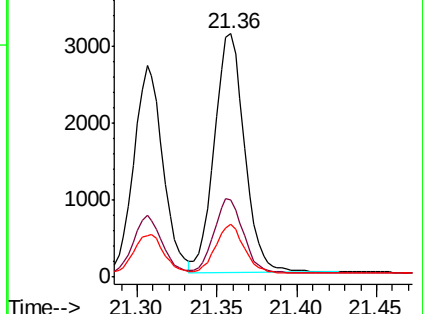

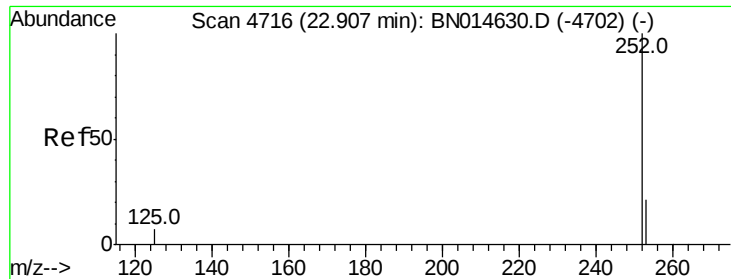

#24

Benzo(b)fluoranthene

Concen: 0.353 ng/ul

RT: 22.90 min Scan# 4715

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38

Instrument :

BNA_N

ClientSampleId :

SLCS090


Tot Ion:252 Resp: 3867

Ion Ratio Lower Upper

252 100

253 26.3 0.0 50.2




125 9.5 0.0 19.4



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

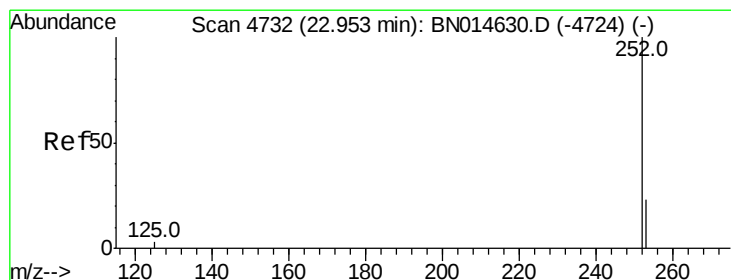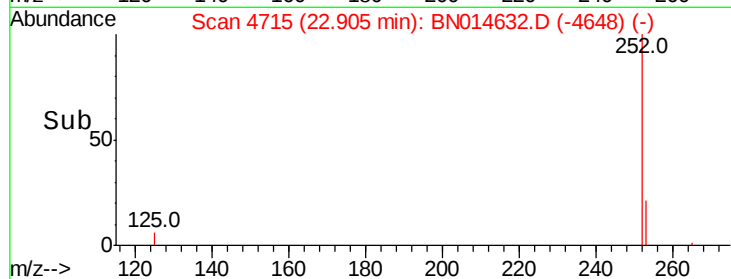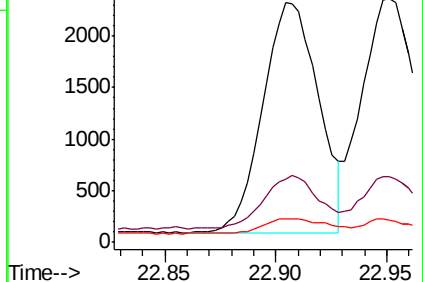

#25

Benzo(k)fluoranthene

Concen: 0.359 ng/ul

RT: 22.95 min Scan# 4731

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38


Tgt Ion:252 Resp: 4149

Ion Ratio Lower Upper

252 100

253 26.7 20.5 30.7



125 9.1 6.9 10.3

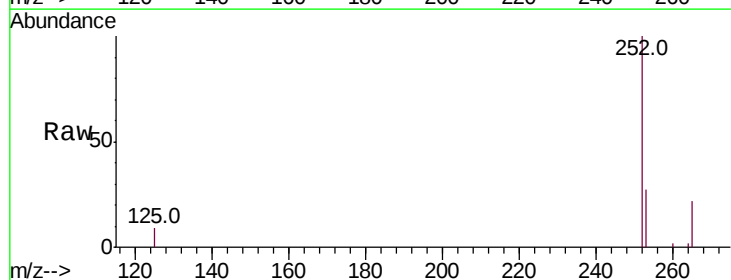


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

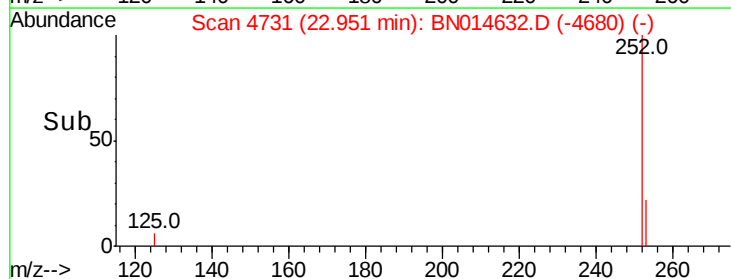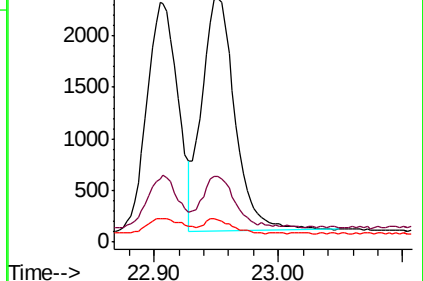

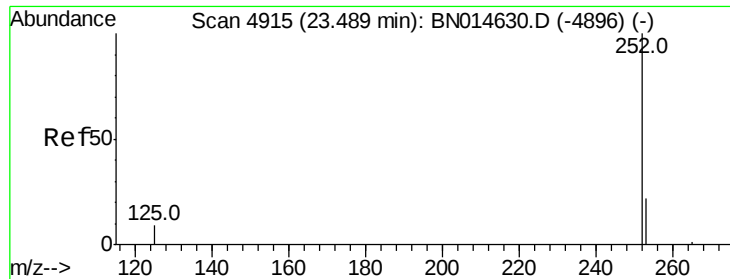

#26

Benzo(a)pyrene

Concen: 0.368 ng/ul

RT: 23.49 min Scan# 4915

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38

Instrument :

BNA_N

ClientSampleId :

SLCS090


Tot Ion:252 Resp: 3082

Ion Ratio Lower Upper

252 100

253 31.9 23.0 34.6




125 13.9 9.5 14.3

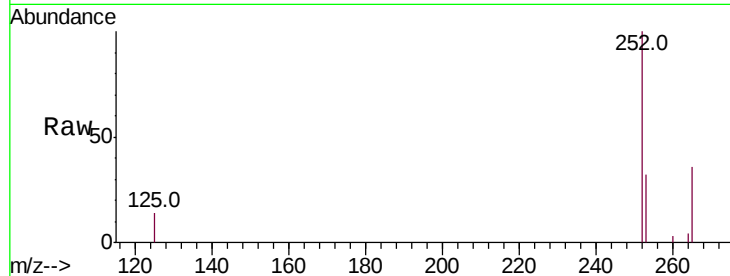

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

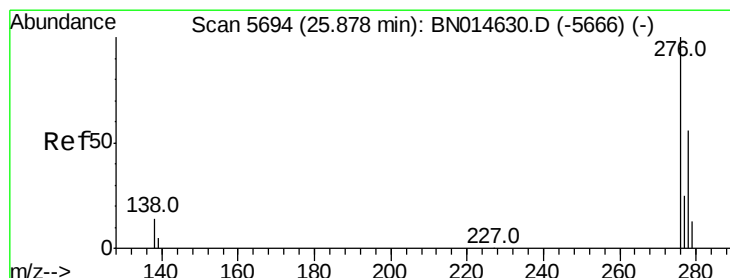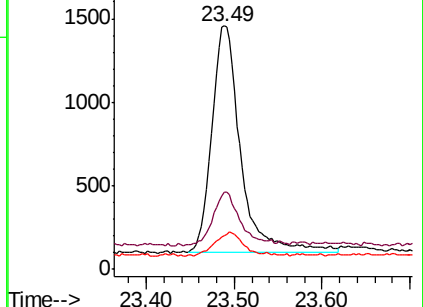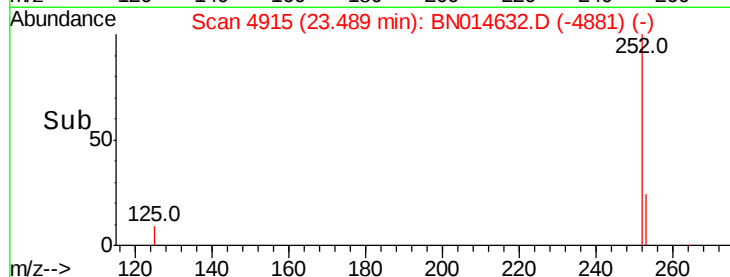

#27

Indeno(1,2,3-cd)pyrene

Concen: 0.375 ng/ul

RT: 25.88 min Scan# 5694

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38


Tgt Ion:276 Resp: 4473

Ion Ratio Lower Upper

276 100

138 13.5 10.9 16.3



227 0.1 0.1 0.1#

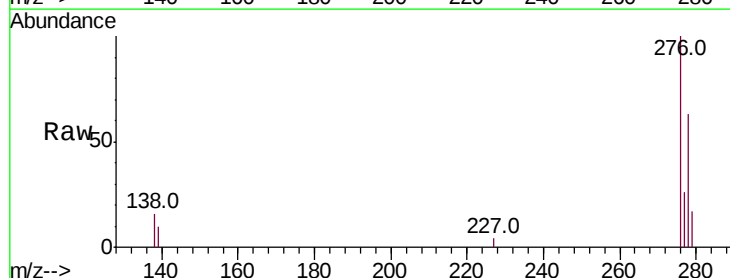


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

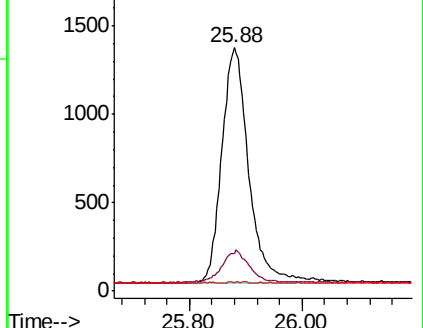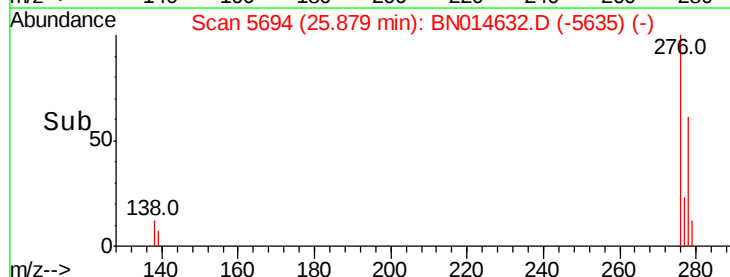



#28

Dibenzo(a,h)anthracene

Concen: 0.377 ng/ul

RT: 25.89 min Scan# 5698

Delta R.T. -0.01 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38

Instrument :

BNA_N

ClientSampleId :

SLCS090


Tot Ion:278 Resp: 3606

Ion Ratio Lower Upper

278 100

139 12.1 10.6 16.0




279 27.9 22.6 34.0

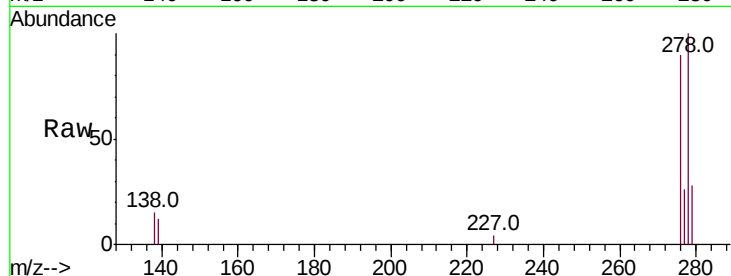

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

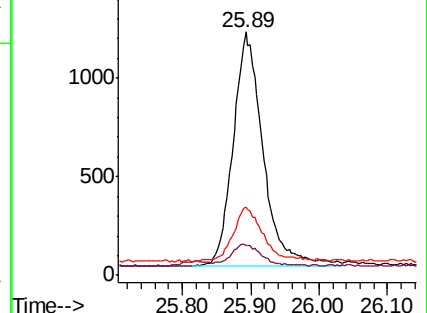

#29

Benzo(g,h,i)perylene

Concen: 0.368 ng/ul

RT: 26.58 min Scan# 5902

Delta R.T. -0.00 min

Lab File: BN014632.D

Acq: 14 May 2021 19:38


Tgt Ion:276 Resp: 3747

Ion Ratio Lower Upper

276 100

138 15.0 11.5 17.3

277 27.4 21.4 32.2



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

