

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN051421\
 Data File : BN014633.D
 Acq On : 14 May 2021 20:49
 Operator : CG/JU
 Sample : M2197-12
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YARH8

Manual Integrations
 APPROVED

mohammad
 5/16/2021 12:16:11 AM

Quant Time: May 14 23:35:39 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 15:50:11 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	379	0.40	ng/ul	0.00
4) Naphthalene-d8	10.52	136	1287	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.38	164	1029	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.13	188	2397m	0.40	ng/ul	0.00
17) Chrysene-d12	21.32	240	2720	0.40	ng/ul	0.00
23) Perylene-d12	23.59	264	2848	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	2069	5.32	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.11	152	876	0.39	ng/ul	0.00
18) Fluoranthene-d10	19.16	212	3354	0.49	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.29	88	88	0.217	ng/ul	Ovalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN051421\
Data File : BN014633.D
Acq On : 14 May 2021 20:49
Operator : CG/JU
Sample : M2197-12
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
YARH8

Quant Time: May 14 23:35:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 15:50:11 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
5/16/2021 12:16:11 AM

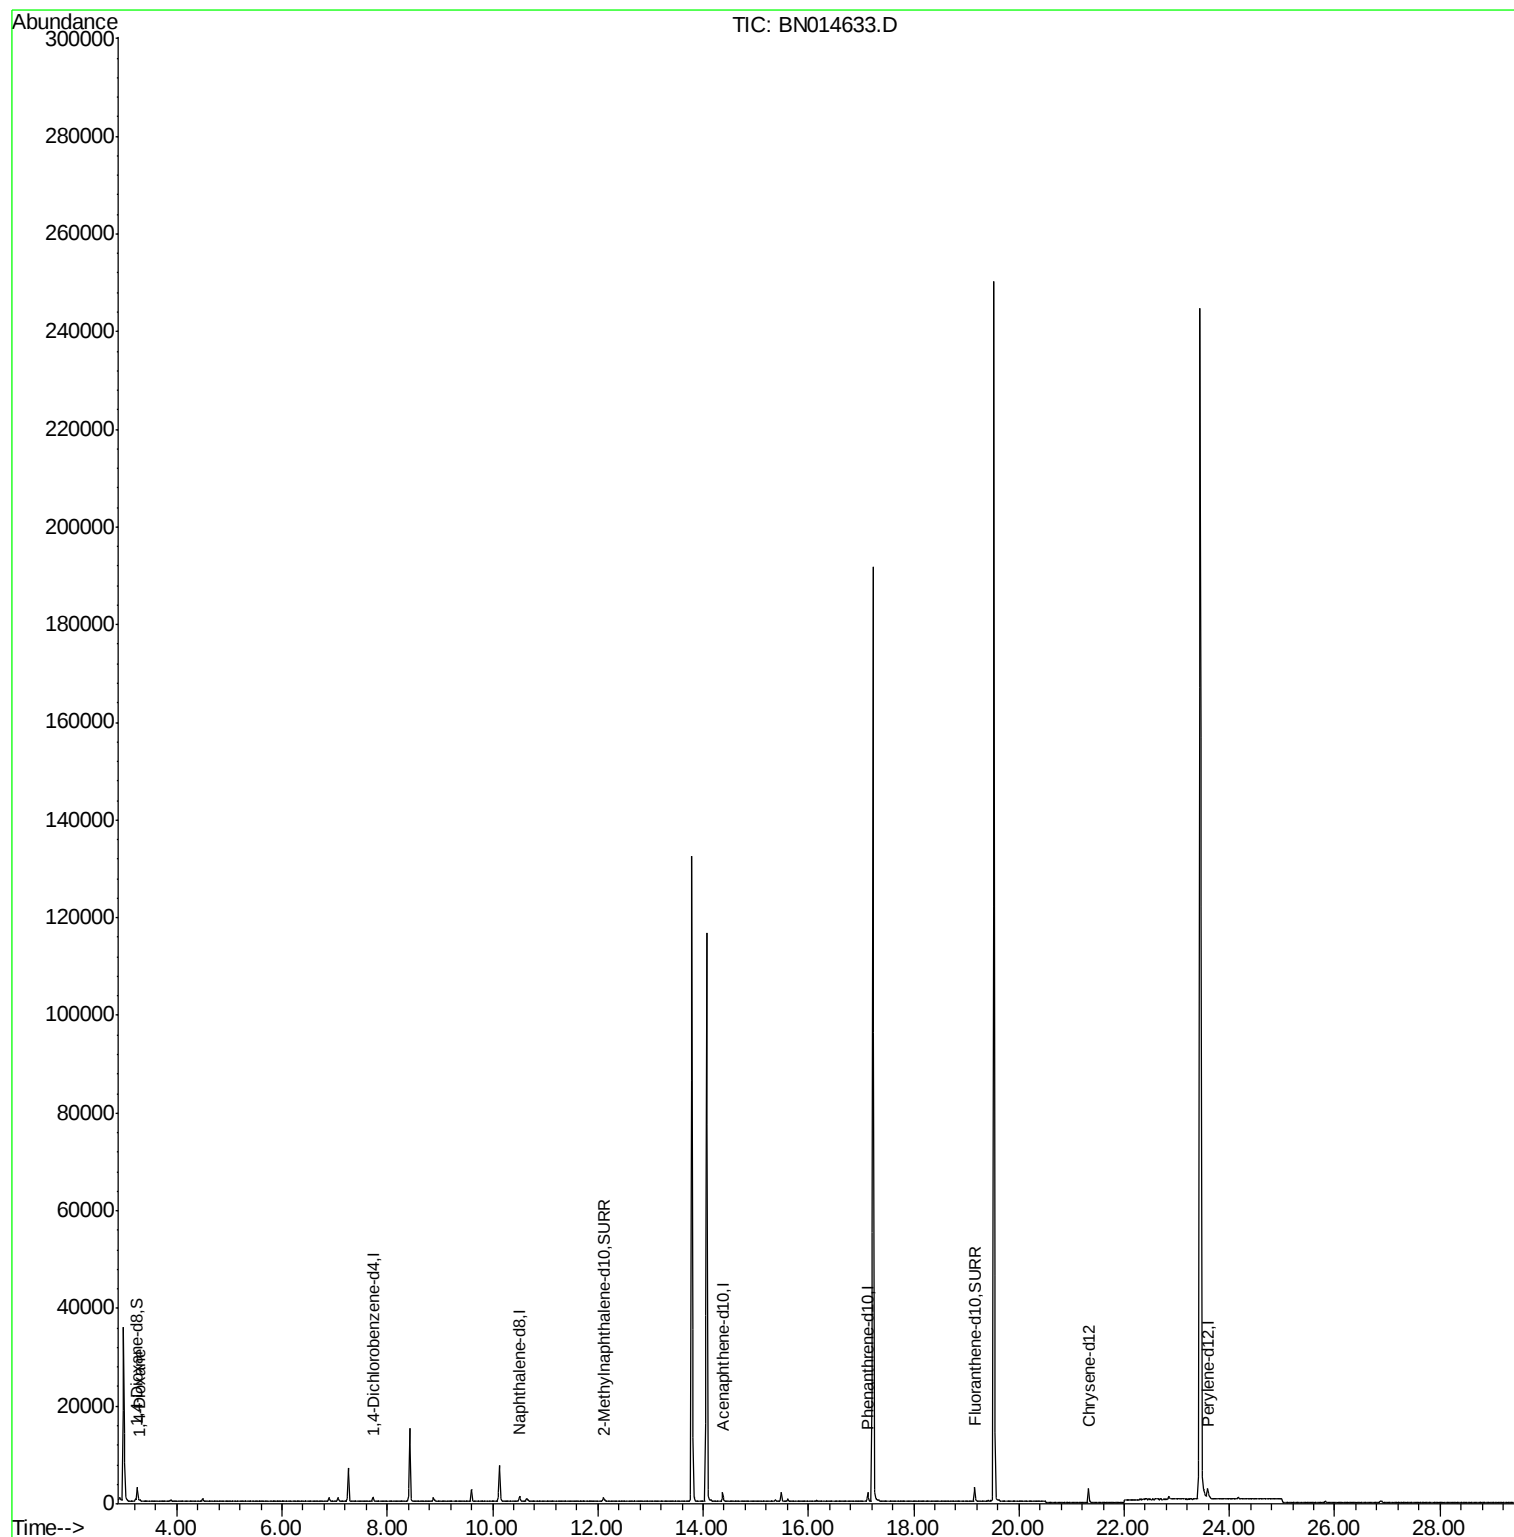

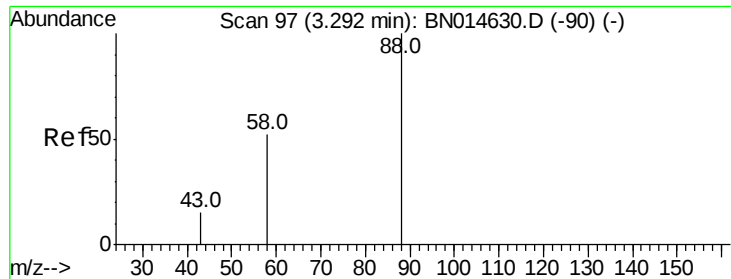

#2

1,4-Dioxane

Concen: 0.217 ng/ul

RT: 3.29 min Scan# 96

Delta R.T. -0.00 min

Lab File: BN014633.D

Acq: 14 May 2021 20:49

Instrument :
BNA_N
ClientSampleId :
YARH8

Tot Ion:	88	Resp:	88
Ion	Ratio	Lower	Upper
88	100		
43	31.9	22.5	33.7
58	35.7	30.4	45.6

Manual Integrations
APPROVED

mohammad
5/16/2021 12:16:11 AM

