
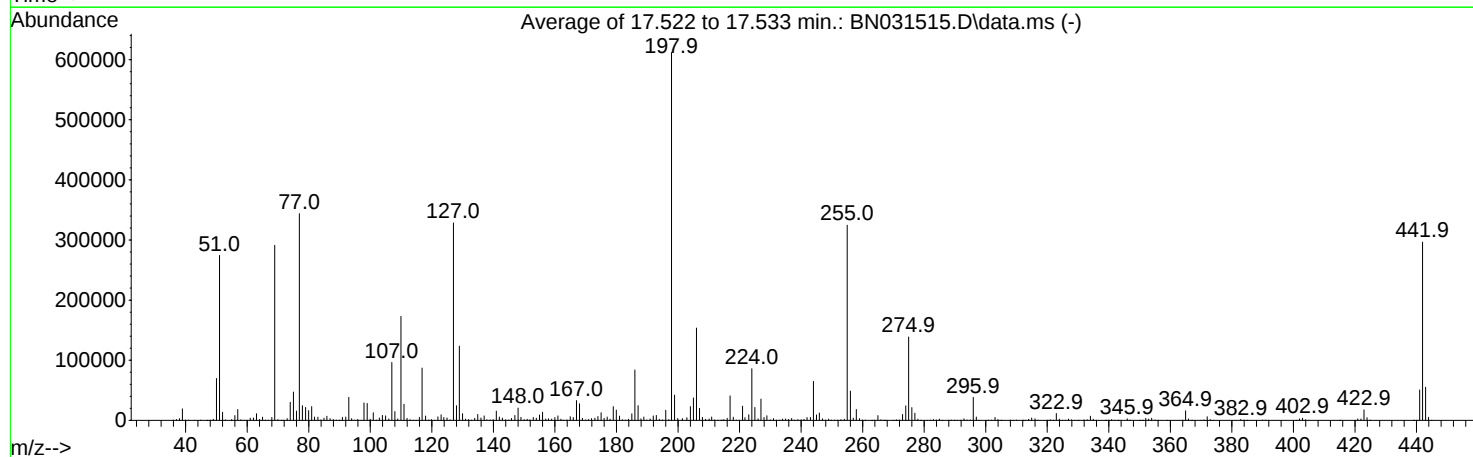


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051424\
Data File : BN031515.D
Acq On : 14 May 2024 08:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 10 02:12:24 2024

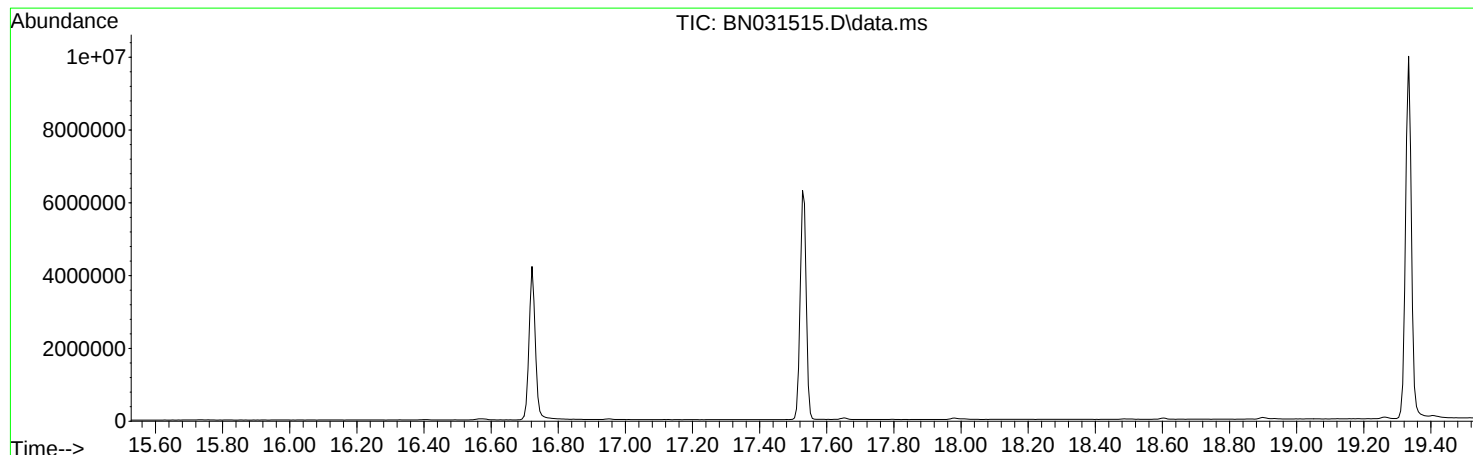

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	274282	PASS
68	69	0.00	2	1.6	4674	PASS
69	198	0.00	100	47.6	291136	PASS
70	69	0.00	2	0.5	1339	PASS
127	198	10	80	53.7	328341	PASS
197	198	0.00	2	0.2	1418	PASS
198	198	100	100	100.0	611883	PASS
199	198	5	9	6.9	42173	PASS
275	198	10	60	22.7	138733	PASS
365	198	1	100	2.6	16017	PASS
441	198	0.01	100	8.3	50504	PASS
442	442	50	100	100.0	296427	PASS
443	442	15	24	18.6	55157	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/14/2024	BNA_N	<u>BN031515.D</u>
Compound Name	Response	Retention Time
DDT	2055279	20.569
DDD	27406	20.127
DDE	1339	19.616
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28745	2084024	1.38

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051424\
Data File : BN031515.D
Acq On : 14 May 2024 08:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 14 11:31:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

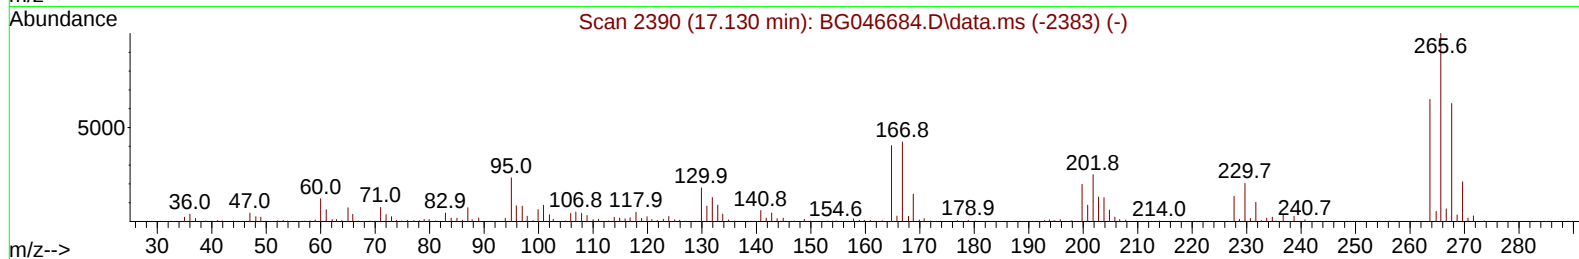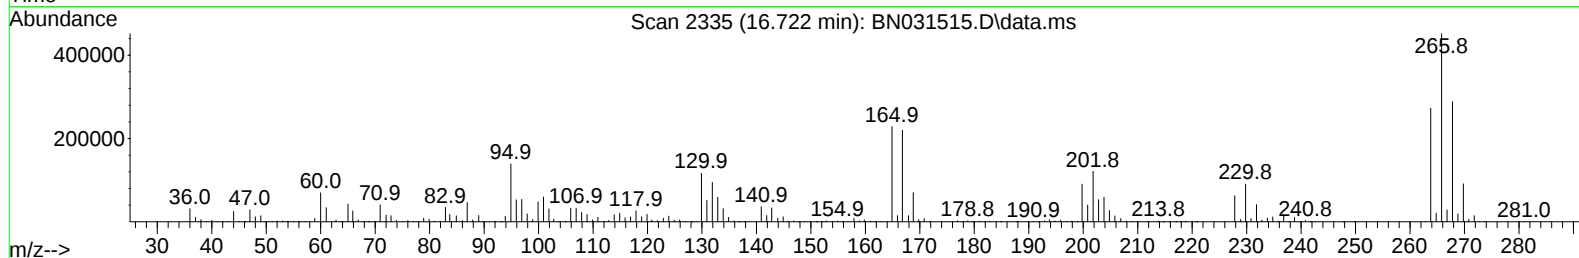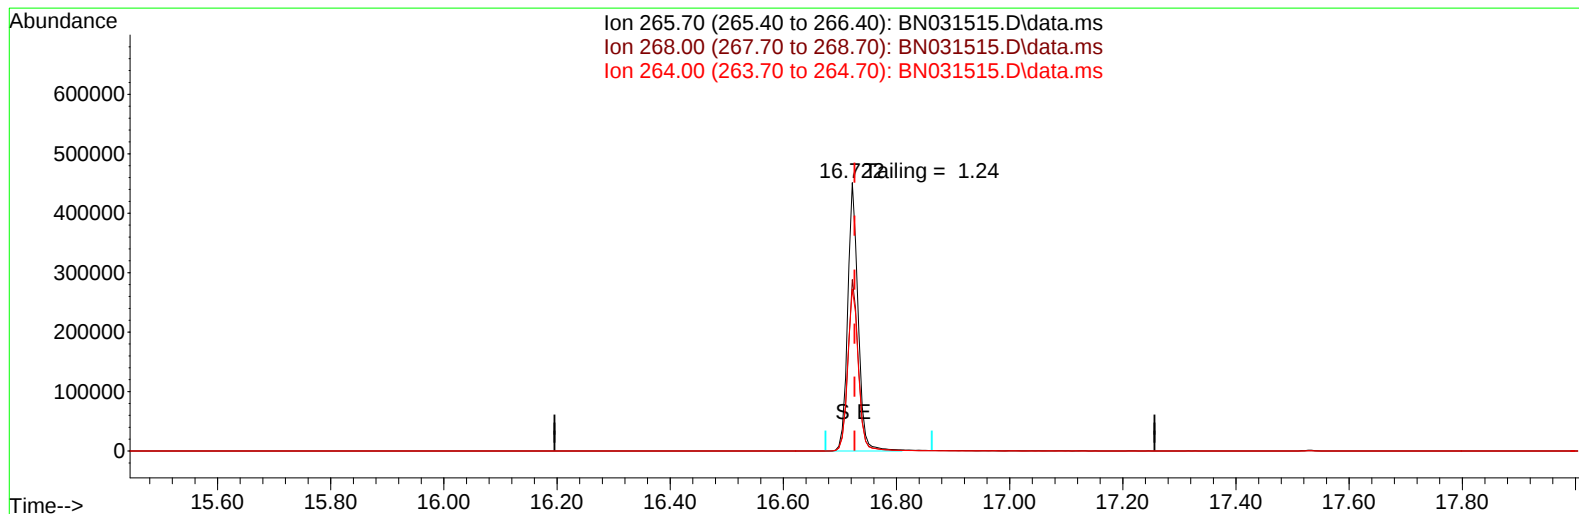

TIC: BN031515.D\data.ms

(70) Pentachlorophenol (C)

16.722min (-0.004) 19243.20 ng




response 582015

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.84
264.00	61.60	60.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051424\
Data File : BN031515.D
Acq On : 14 May 2024 08:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 14 11:31:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

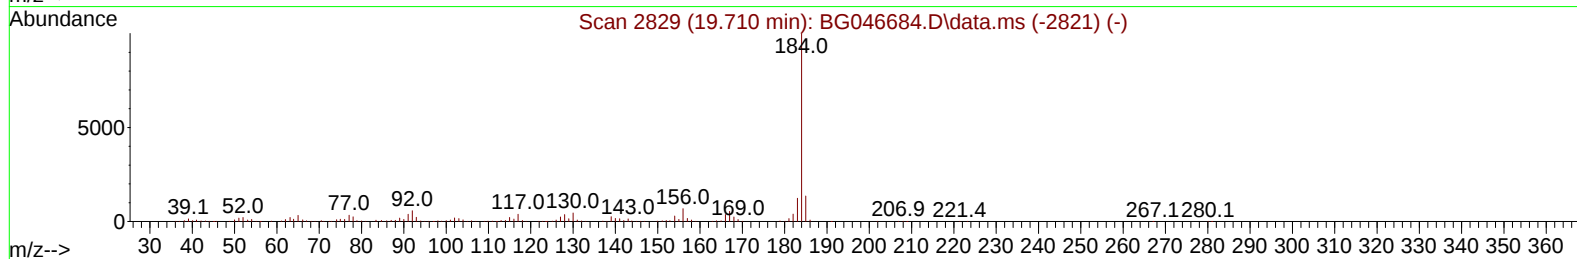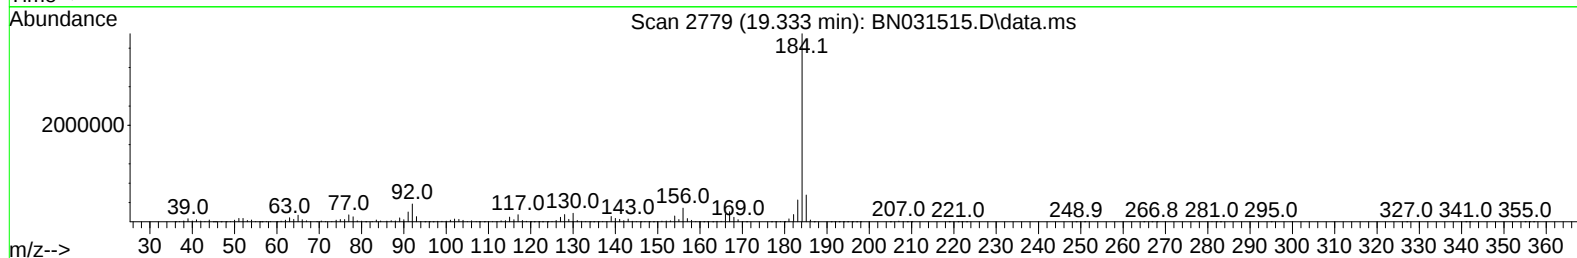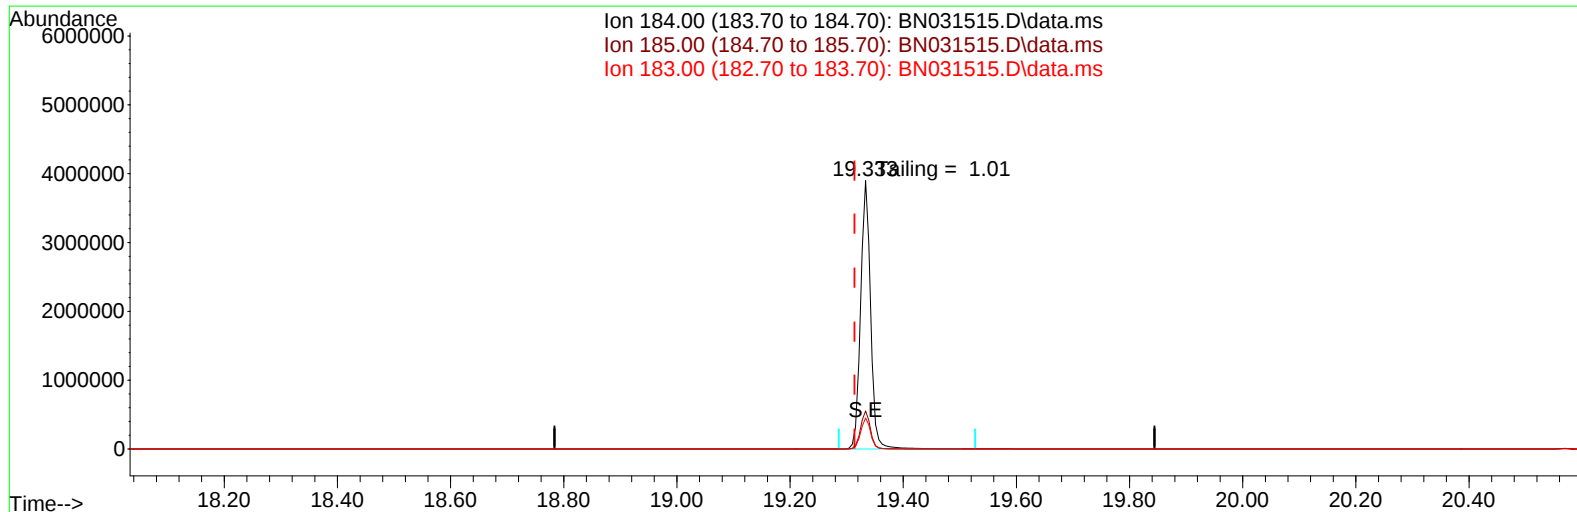

TIC: BN031515.D\data.ms

(77) Benzidine

19.333min (+ 0.019) 0.00 ng

response 4806107

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.23
183.00	13.20	11.59
0.00	0.00	0.00