


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051520\
 Data File : BN010722.D
 Acq On : 15 May 2020 09:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 15 10:34:23 2020

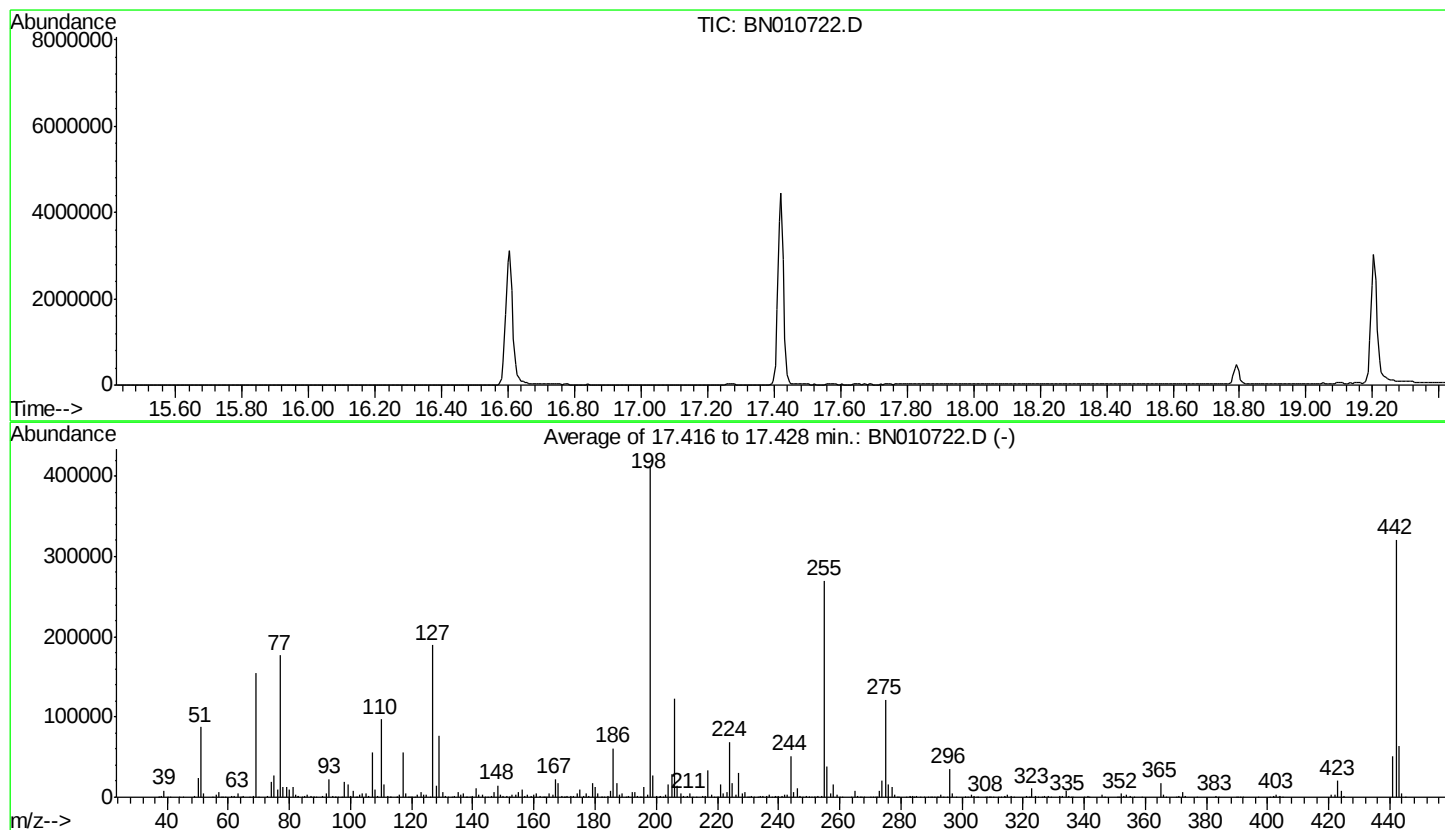

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.2	87445	PASS
68	69	0.00	2	0.7	1145	PASS
69	198	0.00	100	37.3	154221	PASS
70	69	0.00	2	0.5	724	PASS
127	198	10	80	45.9	189482	PASS
197	198	0.00	2	0.6	2600	PASS
198	198	100	100	100.0	413141	PASS
199	198	5	9	6.7	27834	PASS
275	198	10	60	29.4	121410	PASS
365	198	1	100	4.3	17592	PASS
441	198	0.01	100	12.4	51053	PASS
442	198	50	100	77.8	321258	PASS
443	442	15	24	20.0	64309	PASS