
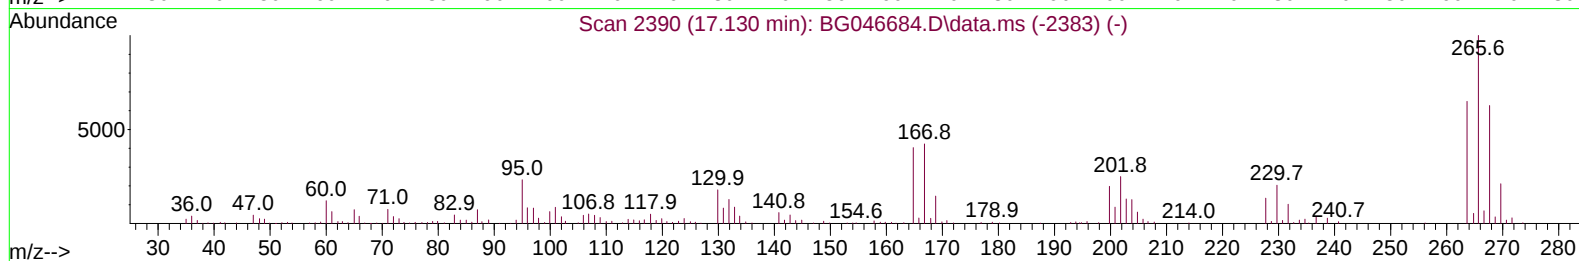
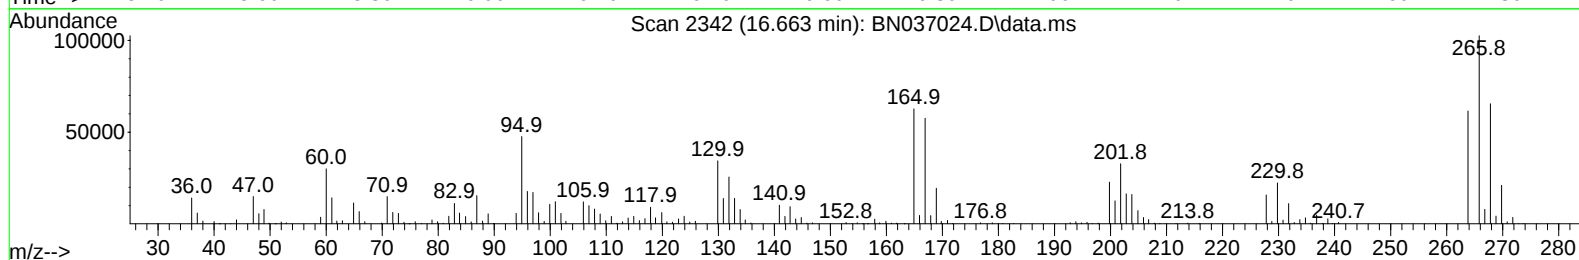


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051525\
Data File : BN037024.D
Acq On : 15 May 2025 09:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 02:43:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 16 02:43:29 2025
Response via : Initial Calibration

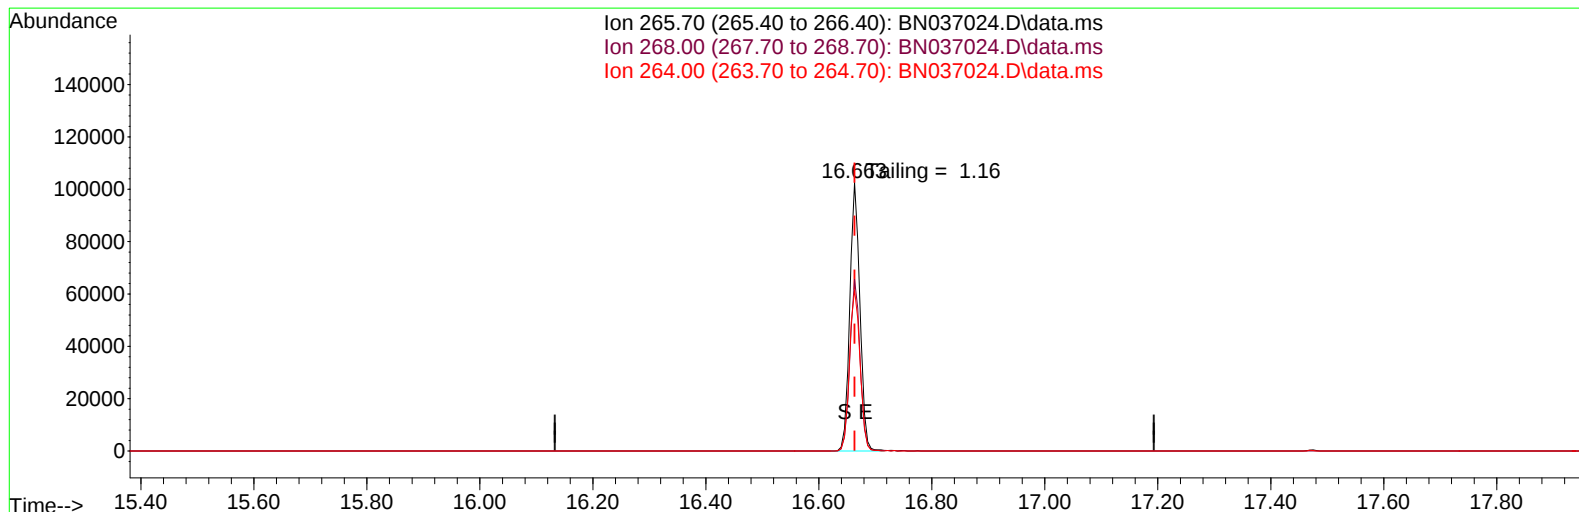

TIC: BN037024.D\data.ms

(70) Pentachlorophenol (C)




16.663min (0.000) 17096.69 ng

response 128267

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.93
264.00	61.60	60.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051525\
Data File : BN037024.D
Acq On : 15 May 2025 09:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 02:43:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 16 02:43:29 2025
Response via : Initial Calibration

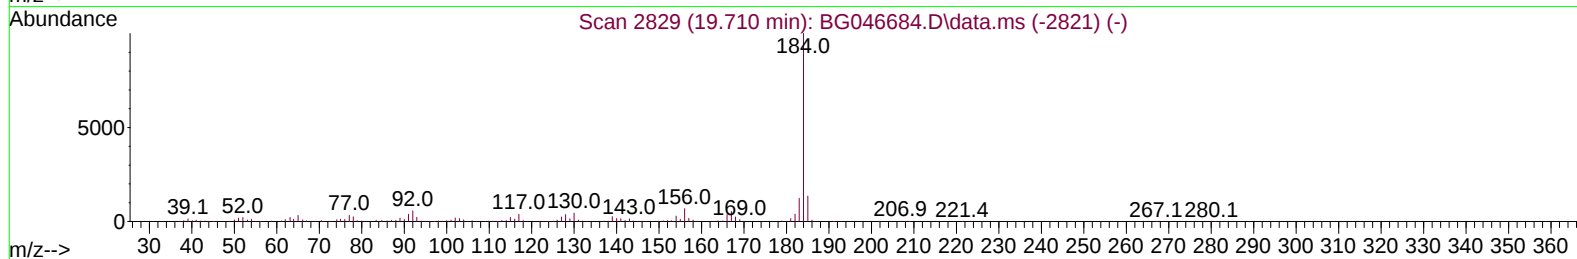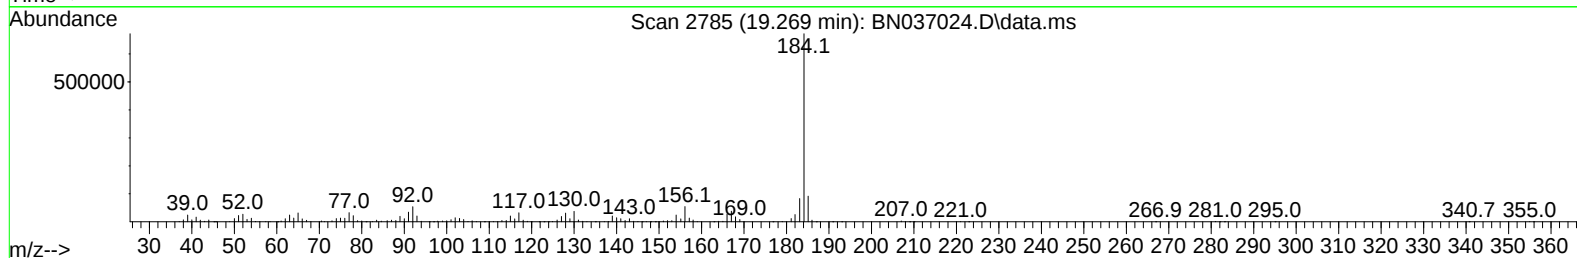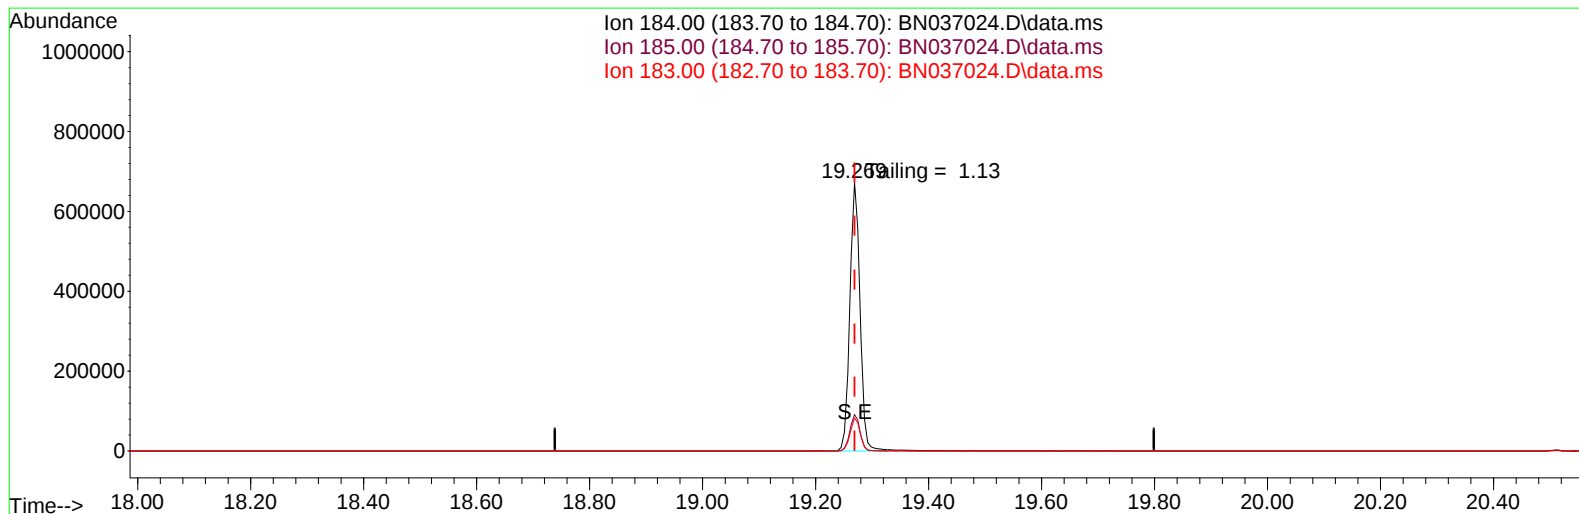

TIC: BN037024.D\data.ms

(77) Benzidine

19.269min (0.000) 0.00 ng

response 850270

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.64
183.00	13.20	12.36
0.00	0.00	0.00