
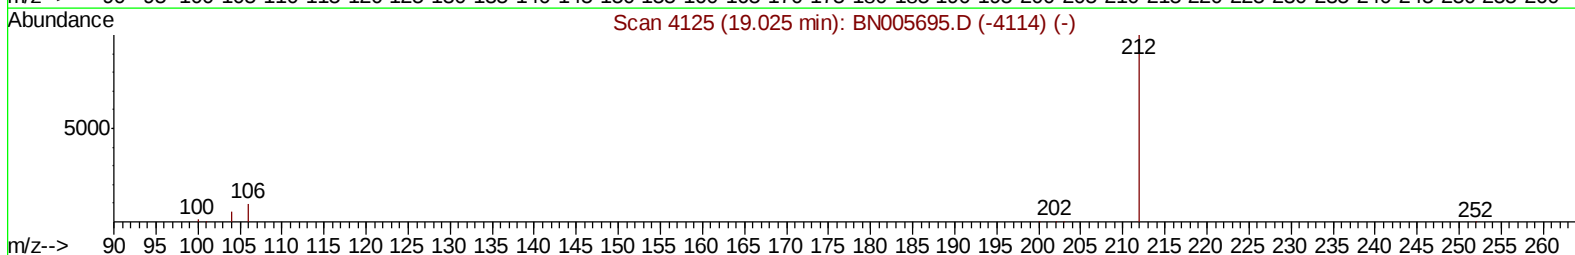
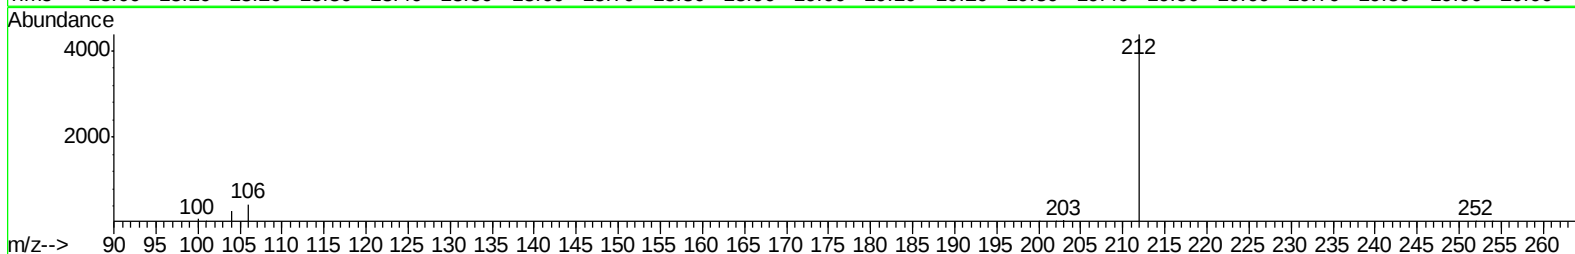


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051619\
Data File : BN005710.D
Acq On : 16 May 2019 19:08
Operator : JU/SJ
Sample : K2788-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: May 17 04:43:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 07:15:06 2019
Response via : Initial Calibration

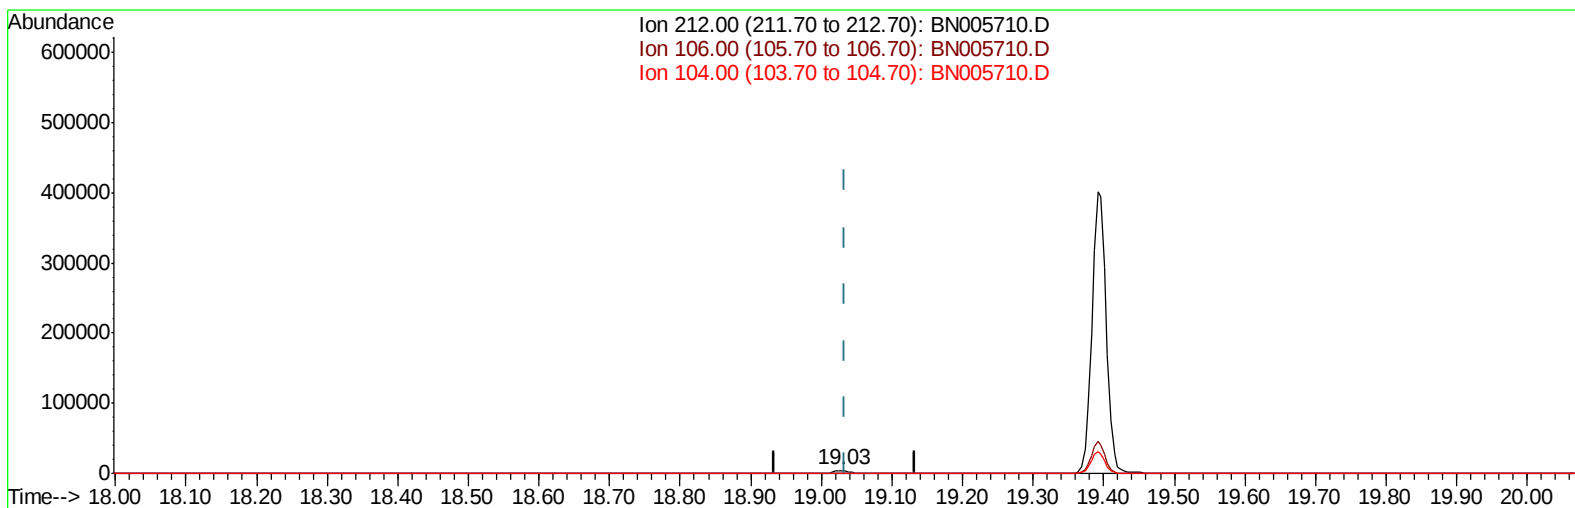

TIC: BN005710.D

(14) Fluoranthene-d10 (SURR)

19.029min (-0.005) 0.31ng/ul m

response 6416

Ion	Exp%	Act%
212.00	100	100
106.00	10.80	0.00#
104.00	6.20	0.00#
0.00	0.00	0.00