
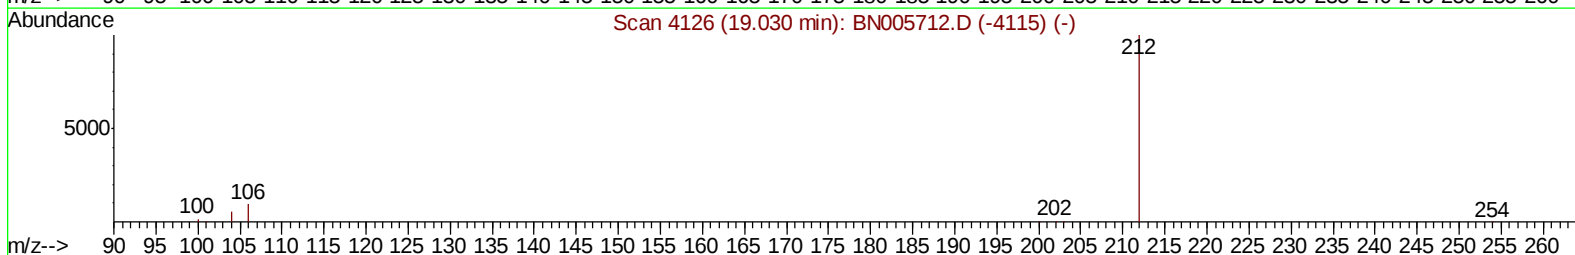
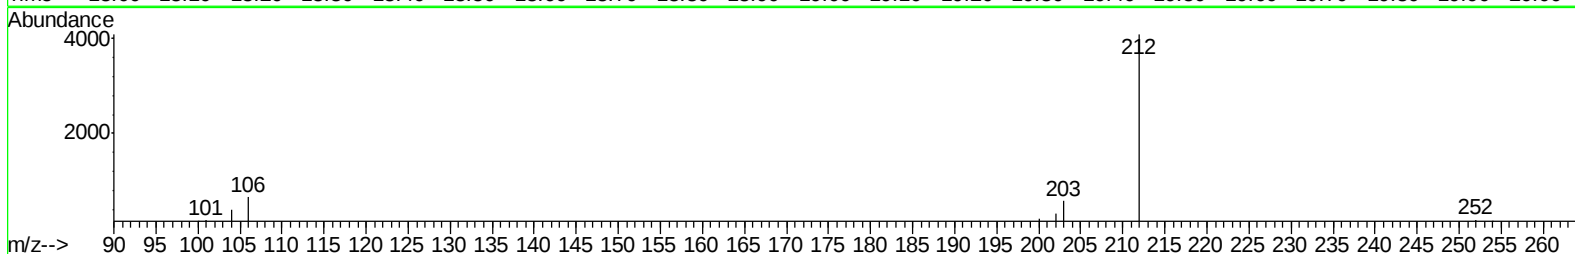


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051619\
Data File : BN005714.D
Acq On : 16 May 2019 22:02
Operator : JU/SJ
Sample : K2690-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: May 17 04:52:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 07:15:06 2019
Response via : Initial Calibration

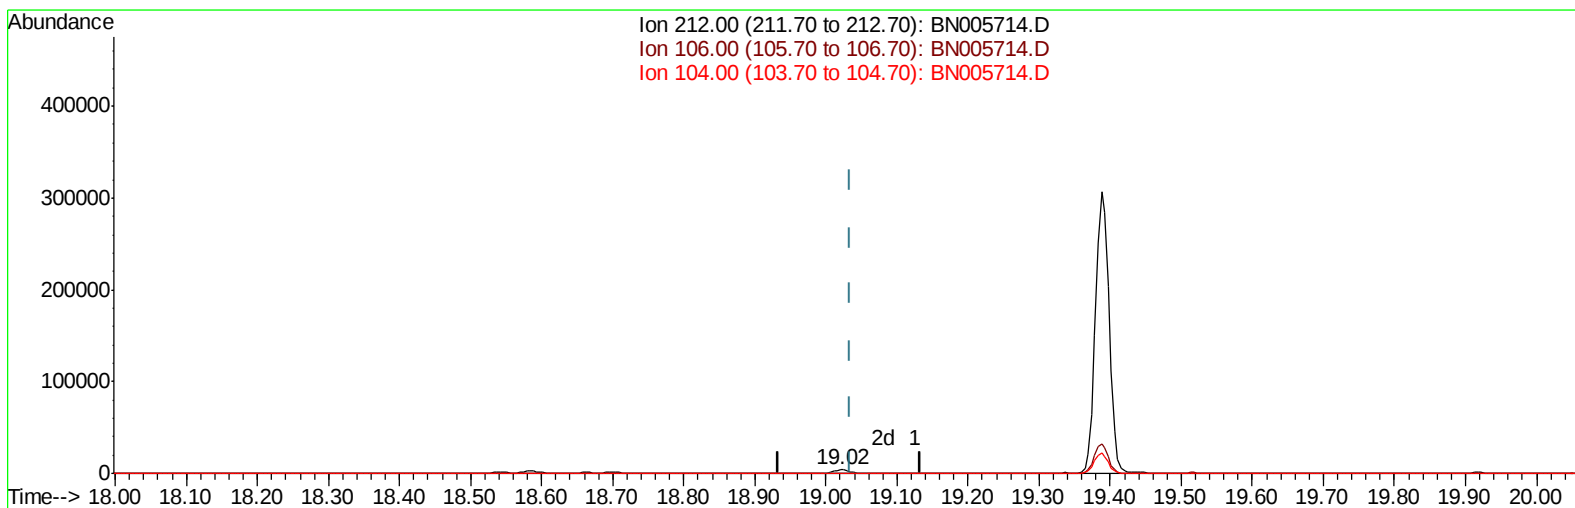

TIC: BN005714.D

(14) Fluoranthene-d10 (SURR)

19.020min (-0.014) 0.19ng/ul m

response 5004

Ion	Exp%	Act%
212.00	100	100
106.00	10.80	0.00#
104.00	6.20	3.18#
0.00	0.00	0.00