
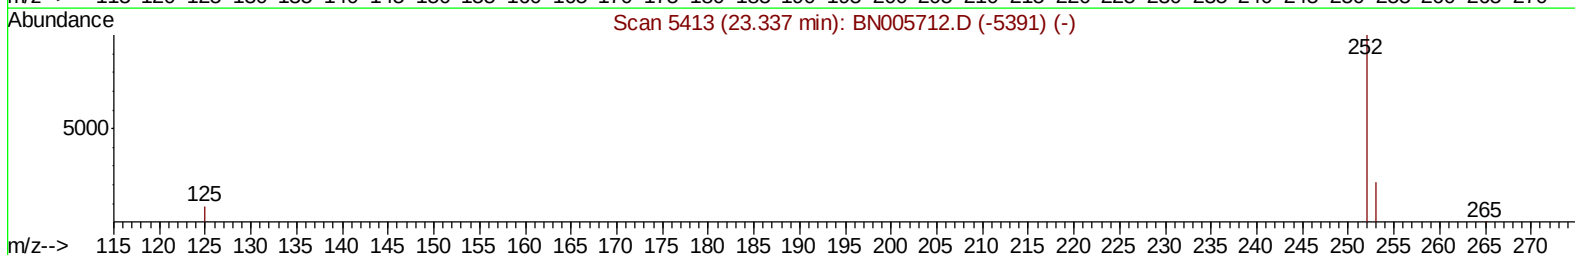
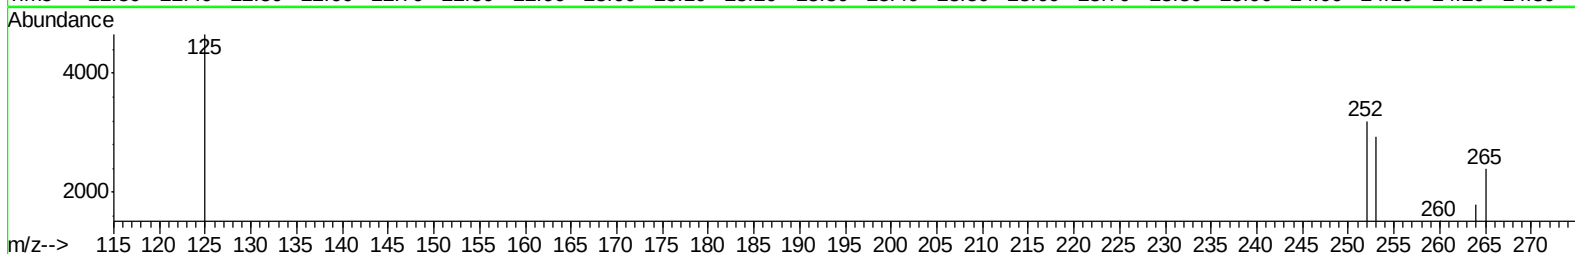


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051619\
Data File : BN005715.D
Acq On : 16 May 2019 22:37
Operator : JU/SJ
Sample : K2690-07DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: May 17 05:03:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 07:15:06 2019
Response via : Initial Calibration

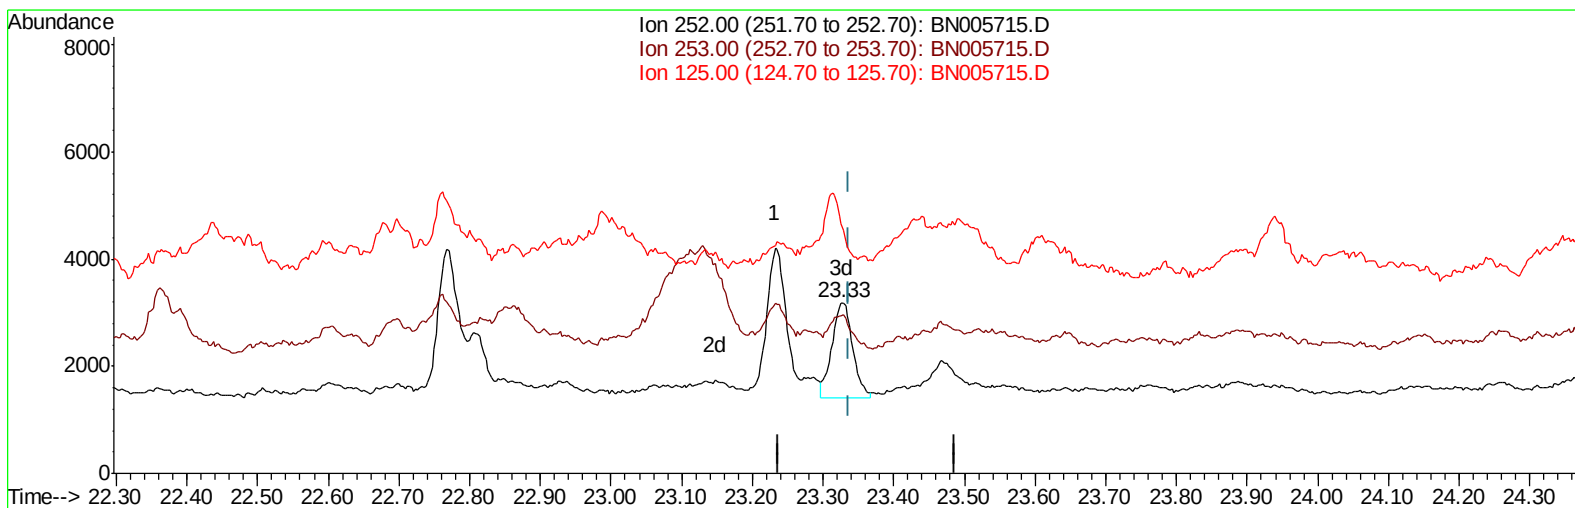

TIC: BN005715.D

(23) Benzo(a)pyrene (C)

23.326min (-0.012) 0.16ng/ul m

response 3556

Ion	Exp%	Act%
252.00	100	100
253.00	24.50	92.12#
125.00	12.60	146.08#
0.00	0.00	0.00