
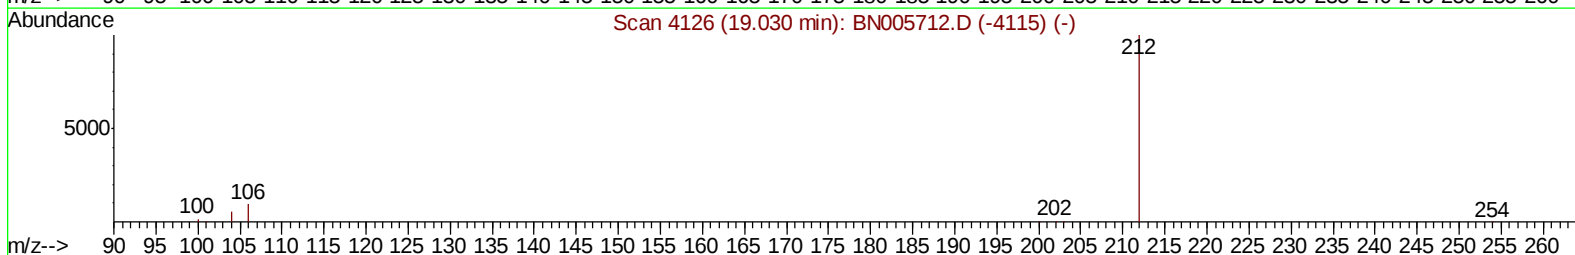
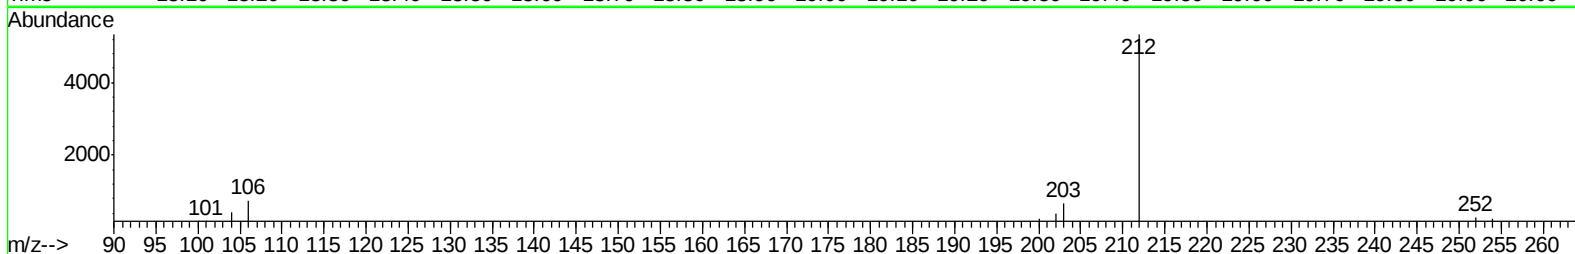


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051619\
Data File : BN005716.D
Acq On : 16 May 2019 23:11
Operator : JU/SJ
Sample : K2690-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: May 17 05:08:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 07:15:06 2019
Response via : Initial Calibration

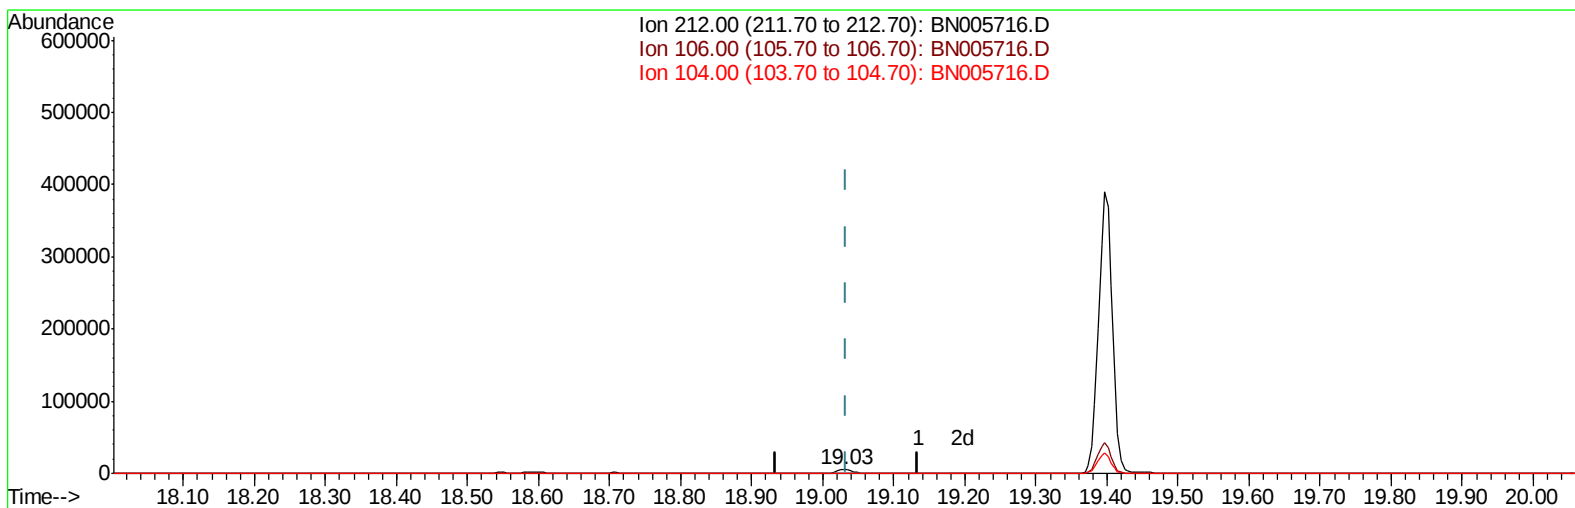

TIC: BN005716.D

(14) Fluoranthene-d10 (SURR)

19.030min (-0.005) 0.22ng/ul m

response 6364

Ion	Exp%	Act%
212.00	100	100
106.00	10.80	0.00#
104.00	6.20	1.05#
0.00	0.00	0.00