
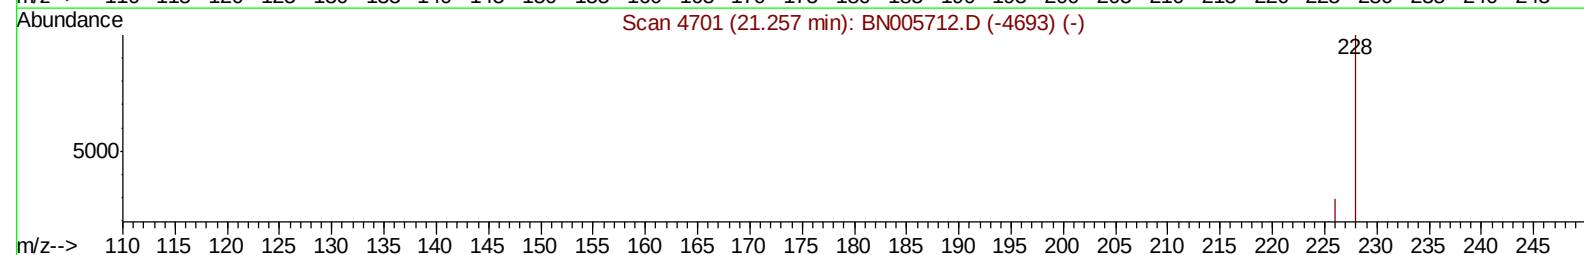
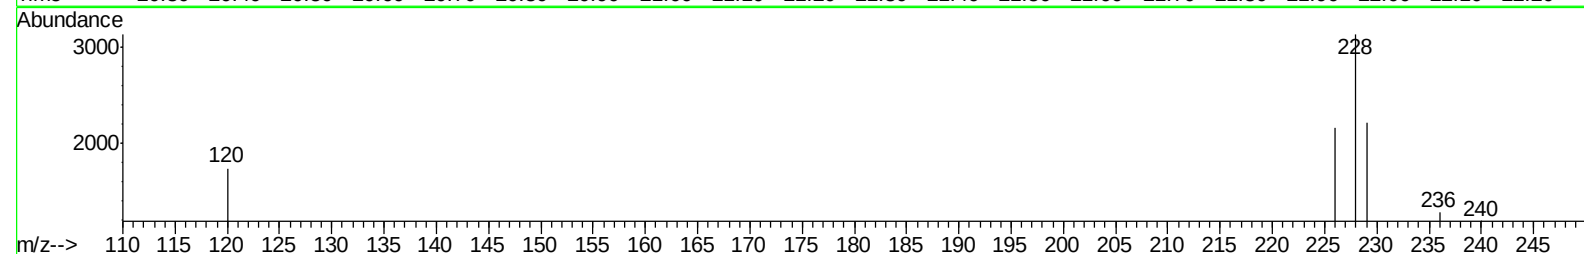


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051619\
 Data File : BN005716.D
 Acq On : 16 May 2019 23:11
 Operator : JU/SJ
 Sample : K2690-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: May 17 05:08:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 14 07:15:06 2019
 Response via : Initial Calibration

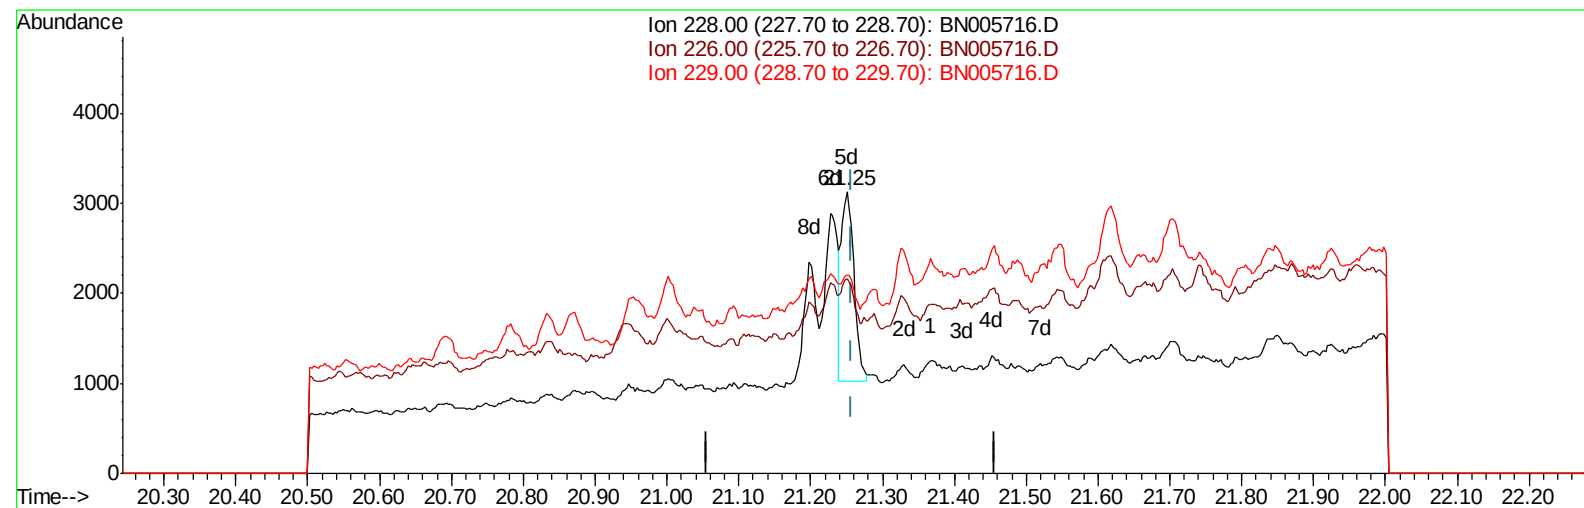

TIC: BN005716.D

(19) Chrysene

21.251min (-0.006) 0.11ng/ul m

response 2553

Ion	Exp%	Act%
228.00	100	100
226.00	29.00	68.91#
229.00	20.00	70.57#
0.00	0.00	0.00