
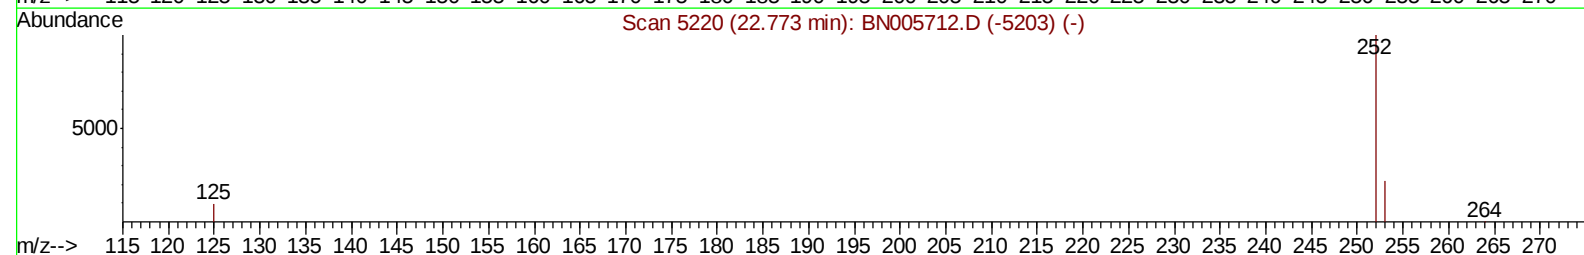
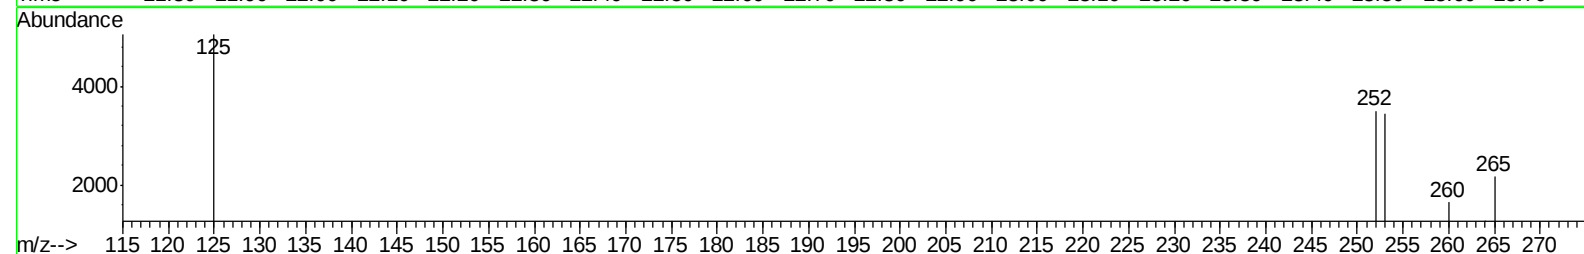


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_N\DATA\BN051619\  
Data File : BN005716.D  
Acq On : 16 May 2019 23:11  
Operator : JU/SJ  
Sample : K2690-14  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Quant Time: May 17 05:08:02 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN050719.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 14 07:15:06 2019  
Response via : Initial Calibration

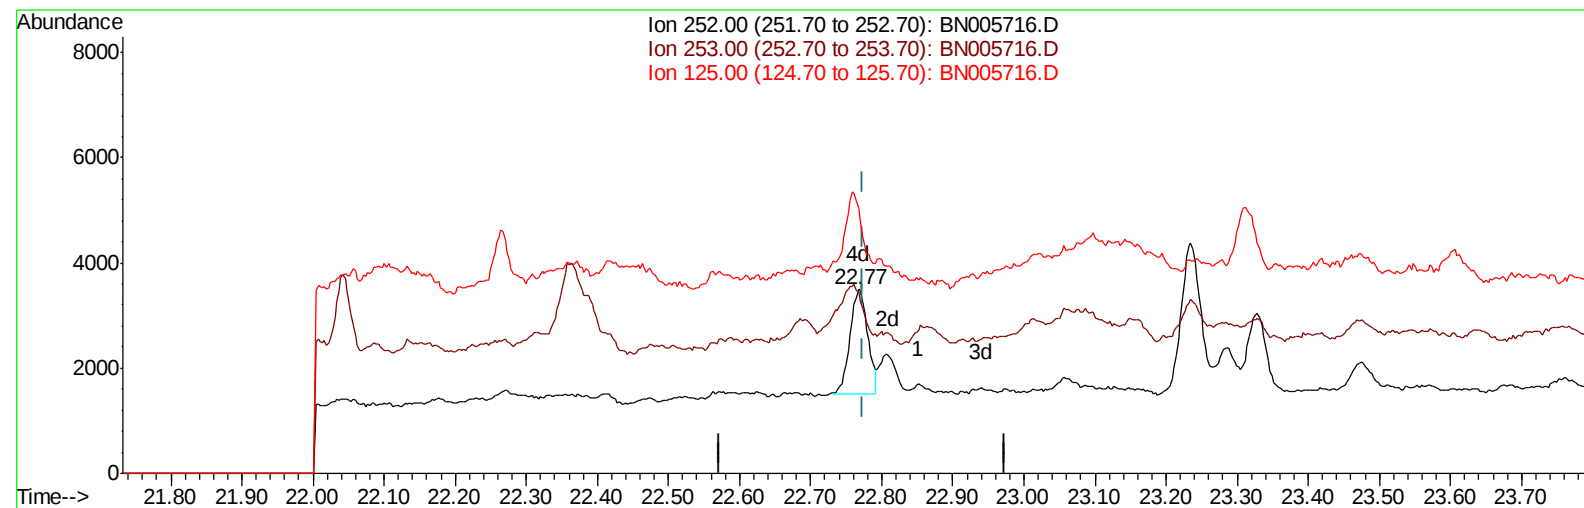

TIC: BN005716.D

(21) Benzo(b)fluoranthene

22.767min (-0.006) 0.21ng/ul m

response 3423

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 252.00 | 100   | 100     |
| 253.00 | 23.80 | 98.37#  |
| 125.00 | 10.40 | 144.16# |
| 0.00   | 0.00  | 0.00    |