
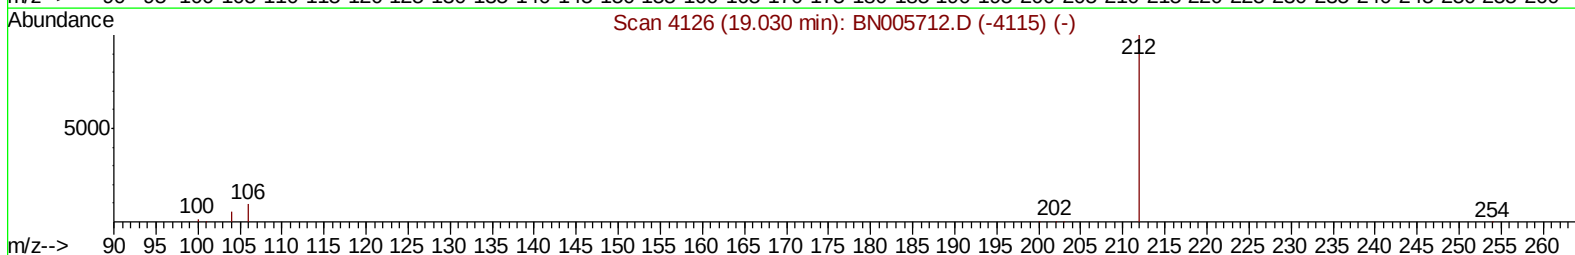
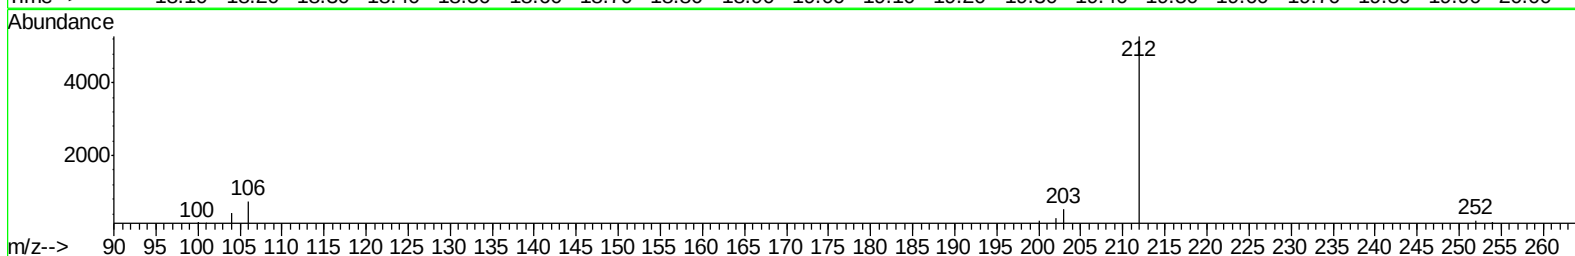


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051619\
Data File : BN005718.D
Acq On : 17 May 2019 00:20
Operator : JU/SJ
Sample : K2690-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: May 17 05:26:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 17 04:47:07 2019
Response via : Initial Calibration

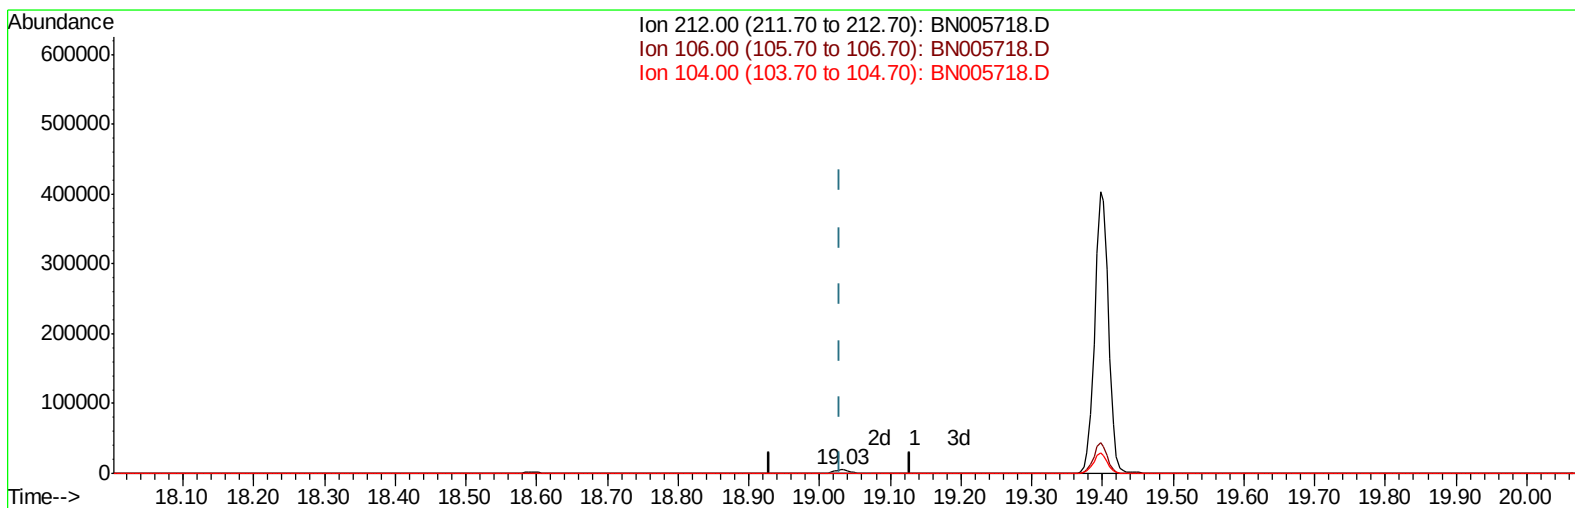

TIC: BN005718.D

(14) Fluoranthene-d10 (SURR)

19.030min (+0.000) 0.26ng/ul m

response 7131

Ion	Exp%	Act%
212.00	100	100
106.00	10.80	0.00#
104.00	6.20	1.11#
0.00	0.00	0.00