
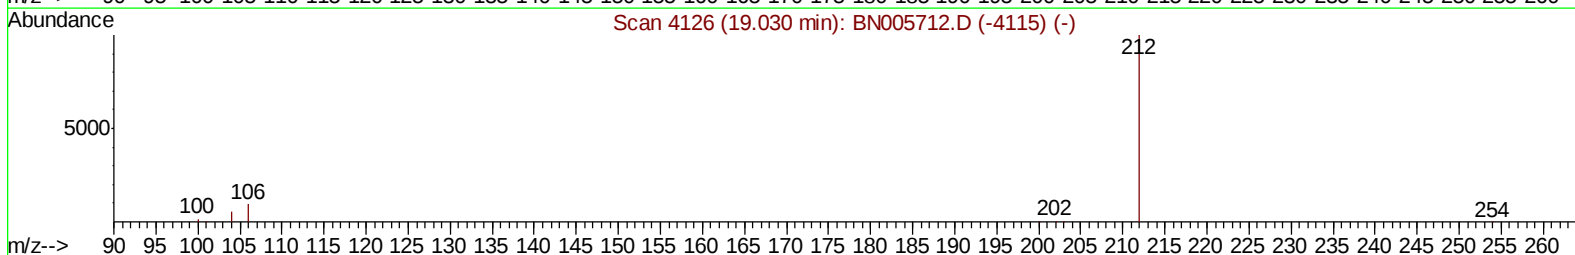
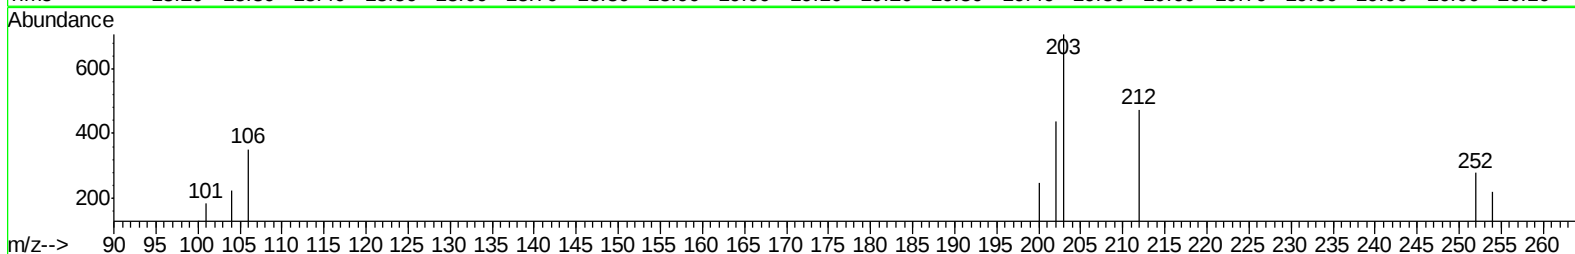


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051619\
 Data File : BN005719.D
 Acq On : 17 May 2019 00:55
 Operator : JU/SJ
 Sample : K2690-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: May 17 05:53:31 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 14 07:15:06 2019
 Response via : Initial Calibration

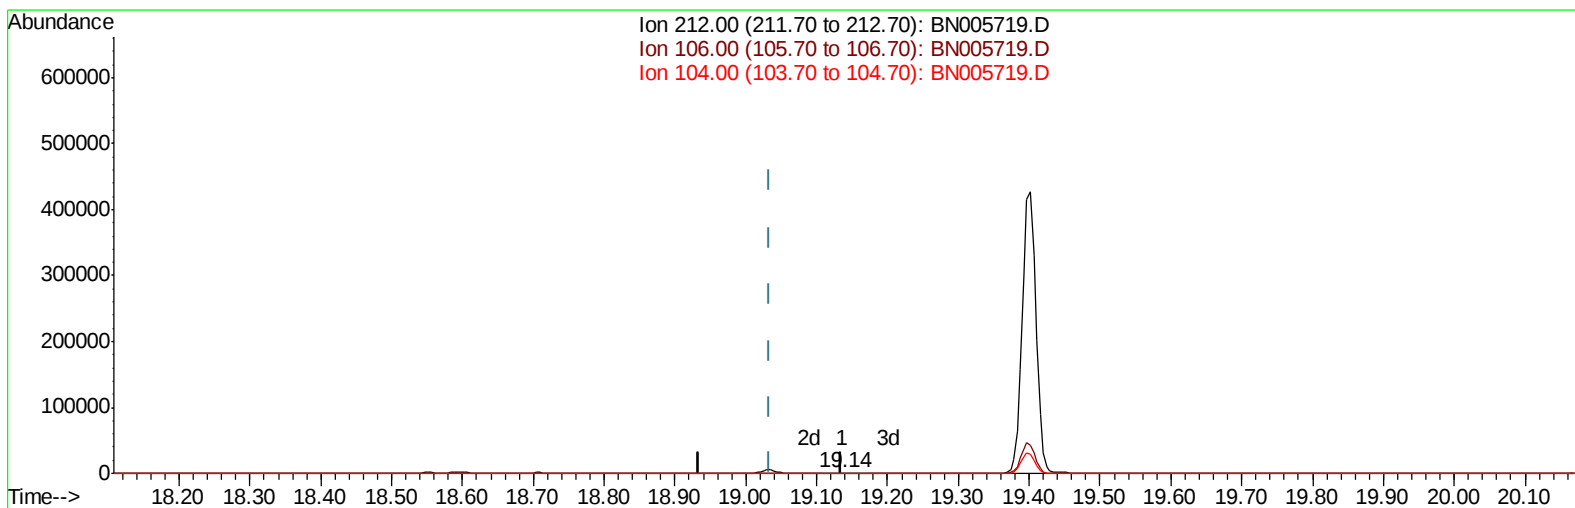

TIC: BN005719.D

(14) Fluoranthene-d10 (SURR)

19.137min (+0.102) 0.01ng/ul

response 406

Ion	Exp%	Act%
212.00	100	100
106.00	10.80	8.87
104.00	6.20	20.20#
0.00	0.00	0.00