
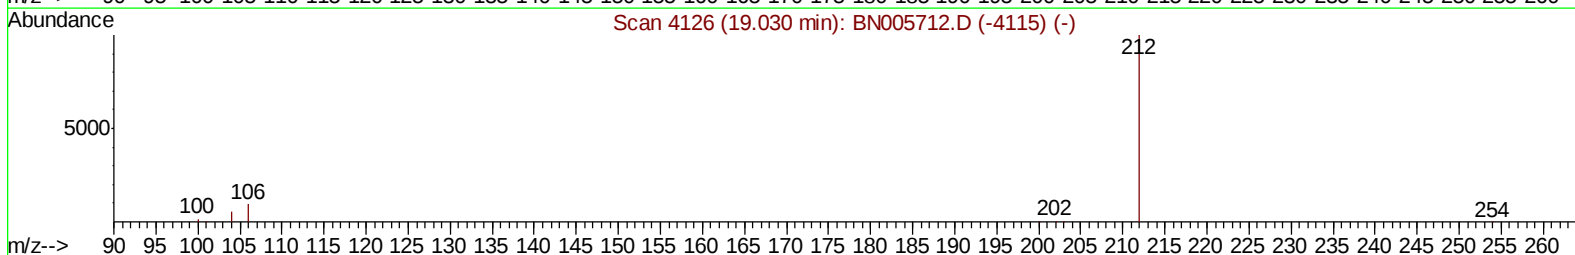
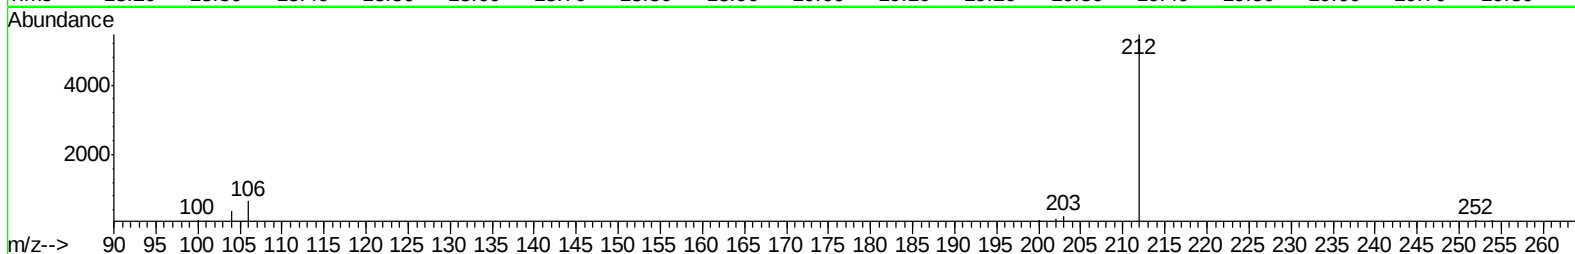


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051619\
Data File : BN005722.D
Acq On : 17 May 2019 02:38
Operator : JU/SJ
Sample : K2788-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: May 17 06:32:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 17 04:47:07 2019
Response via : Initial Calibration

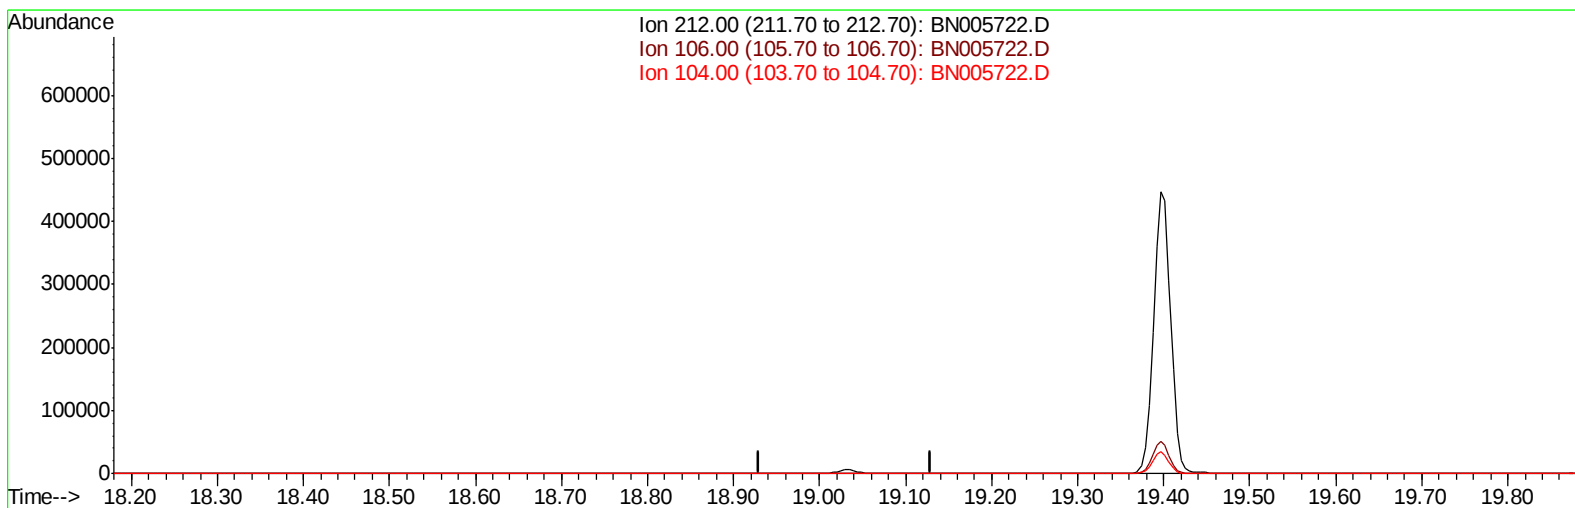

TIC: BN005722.D

(14) Fluoranthene-d10 (SURR)

19.030min (-19.030) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	10.80	0.00#
104.00	6.20	0.00#
0.00	0.00	0.00