

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051619\
 Data File : BN005711.D
 Acq On : 16 May 2019 19:43
 Operator : JU/SJ
 Sample : K2788-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5192

Quant Time: May 17 04:39:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 14 07:15:06 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	738	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.35	136	3234	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.22	164	2124	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.08	188	371898	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.22
20) Perylene-d12	23.28	264	487549	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	1449	0.29	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.22	166	546	0.062	ng/ul#	Qvalue 20


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051619\
Data File : BN005711.D
Acq On : 16 May 2019 19:43
Operator : JU/SJ
Sample : K2788-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5192

Quant Time: May 17 04:39:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 07:15:06 2019
Response via : Initial Calibration

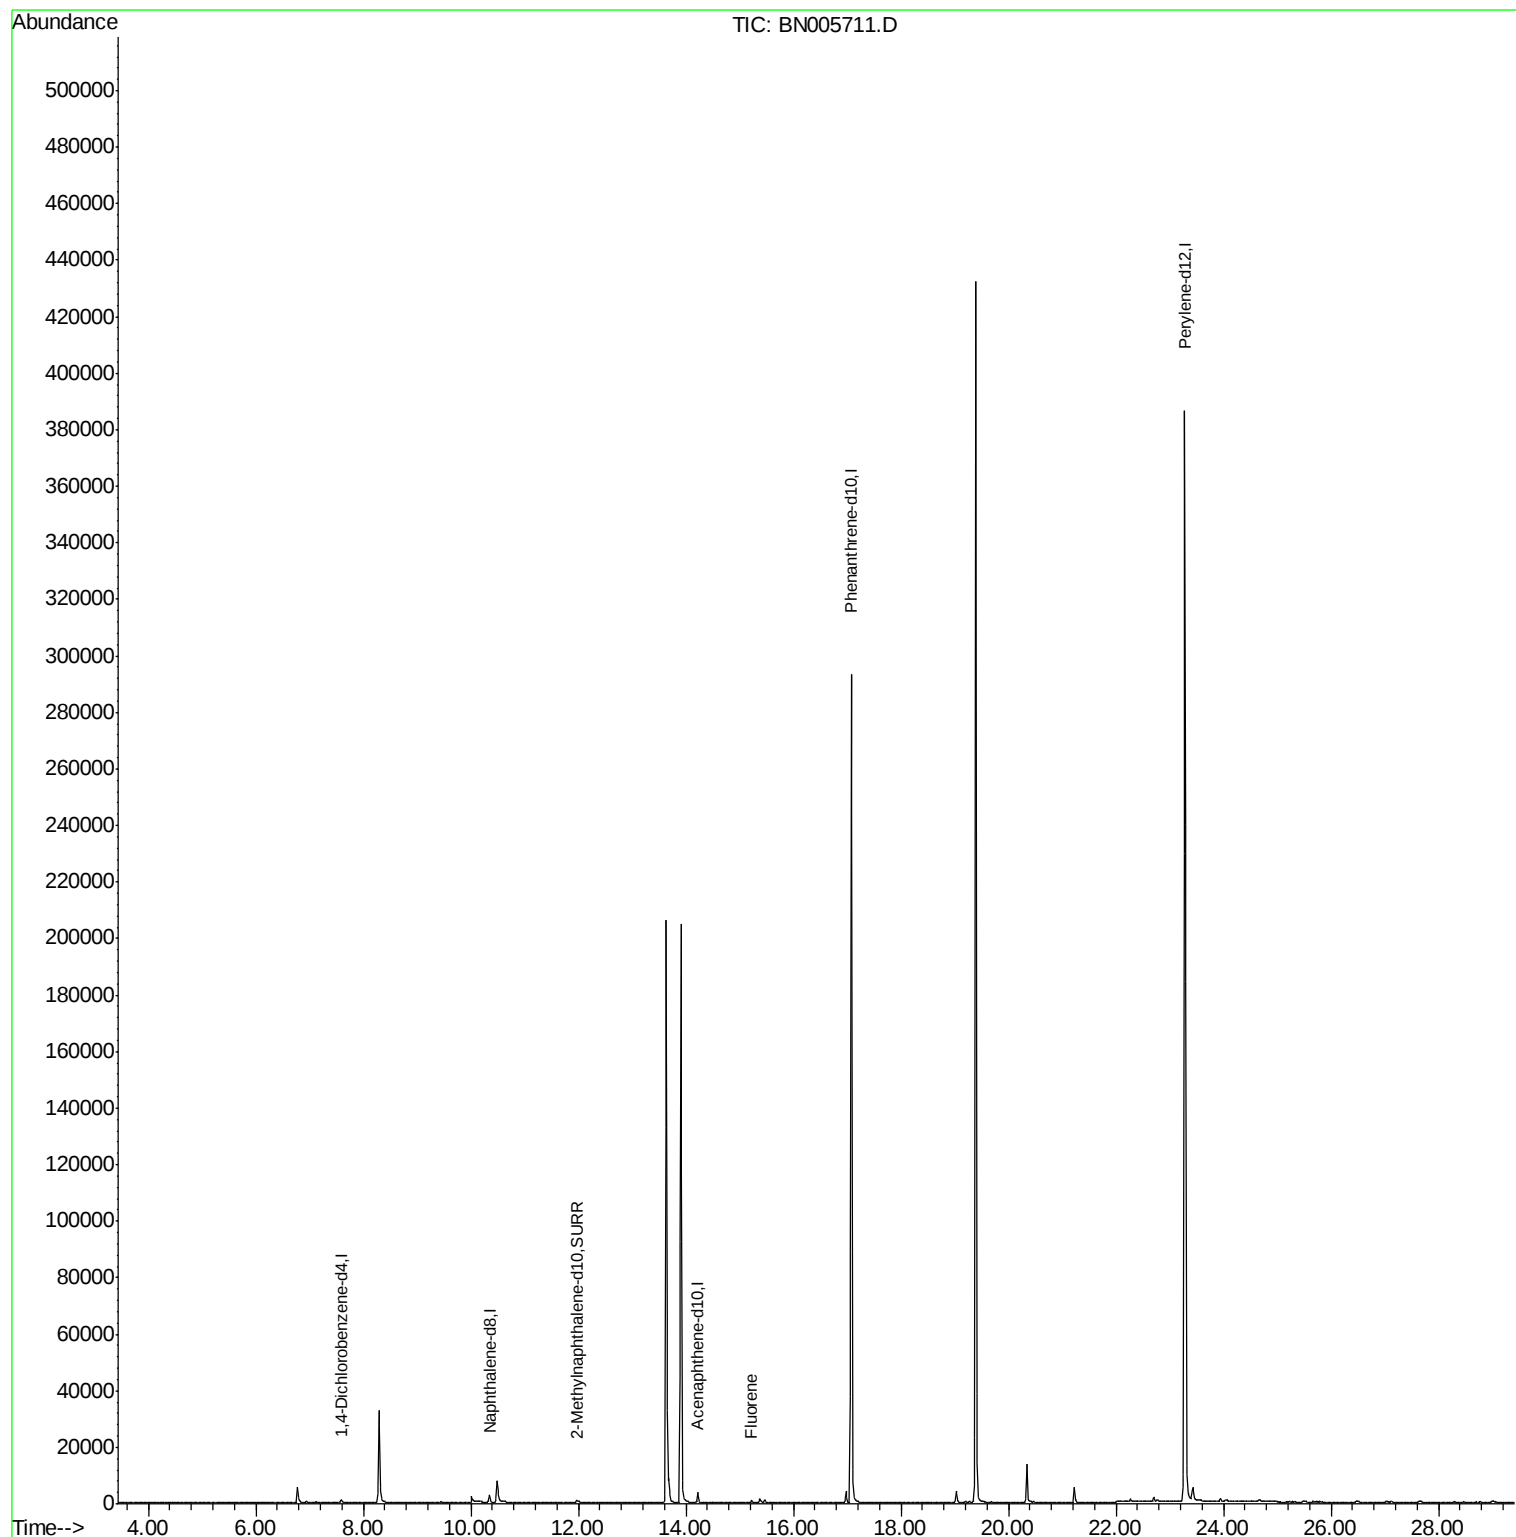

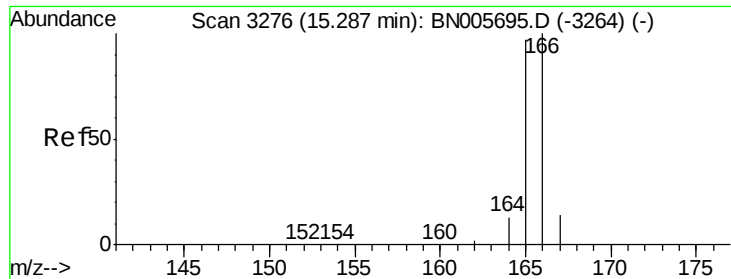

#9

Fluorene

Concen: 0.062 ng/ul

RT: 15.22 min Scan# 3262

Delta R.T. -0.07 min

Lab File: BN005711.D

Acq: 16 May 2019 19:43

Instrument :

BNA_N

ClientSampleId :

A5192


Tgt Ion:166 Resp: 546

Ion Ratio Lower Upper

166 100

165 16.1 78.0 117.0#

167 42.0 12.2 18.4#

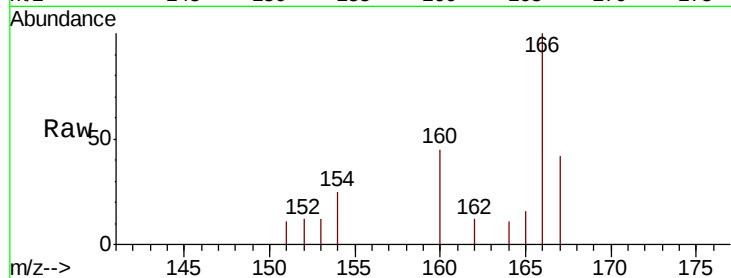

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

