

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN051619\
 Data File : BN005707.D
 Acq On : 16 May 2019 17:25
 Operator : JU/SJ
 Sample : K2690-23MSD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5167MSD

Quant Time: May 16 18:36:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN050719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 14 07:15:06 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	661	0.40	ng/ul	0.00
2) Naphthalene-d8	10.37	136	2830	0.40	ng/ul	0.02
6) Acenaphthene-d10	14.22	164	2023	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	5080	0.40	ng/ul	0.00
16) Chrysene-d12	21.24	240	5912	0.40	ng/ul	0.02
20) Perylene-d12	23.46	264	6378	0.40	ng/ul	0.04
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.98	152	1762	0.40	ng/ul	0.02
14) Fluoranthene-d10	19.03	212	6412	0.40	ng/ul	0.00
Target Compounds				Ovalue		
8) Acenaphthene	14.28	153	2406	0.334	ng/ul	97
11) Pentachlorophenol	16.70	266	334	0.254	ng/ul#	80
17) Pyrene	19.43	202	7643	0.350	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN051619\
Data File : BN005707.D
Acq On : 16 May 2019 17:25
Operator : JU/SJ
Sample : K2690-23MSD
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5167MSD

Quant Time: May 16 18:36:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 07:15:06 2019
Response via : Initial Calibration

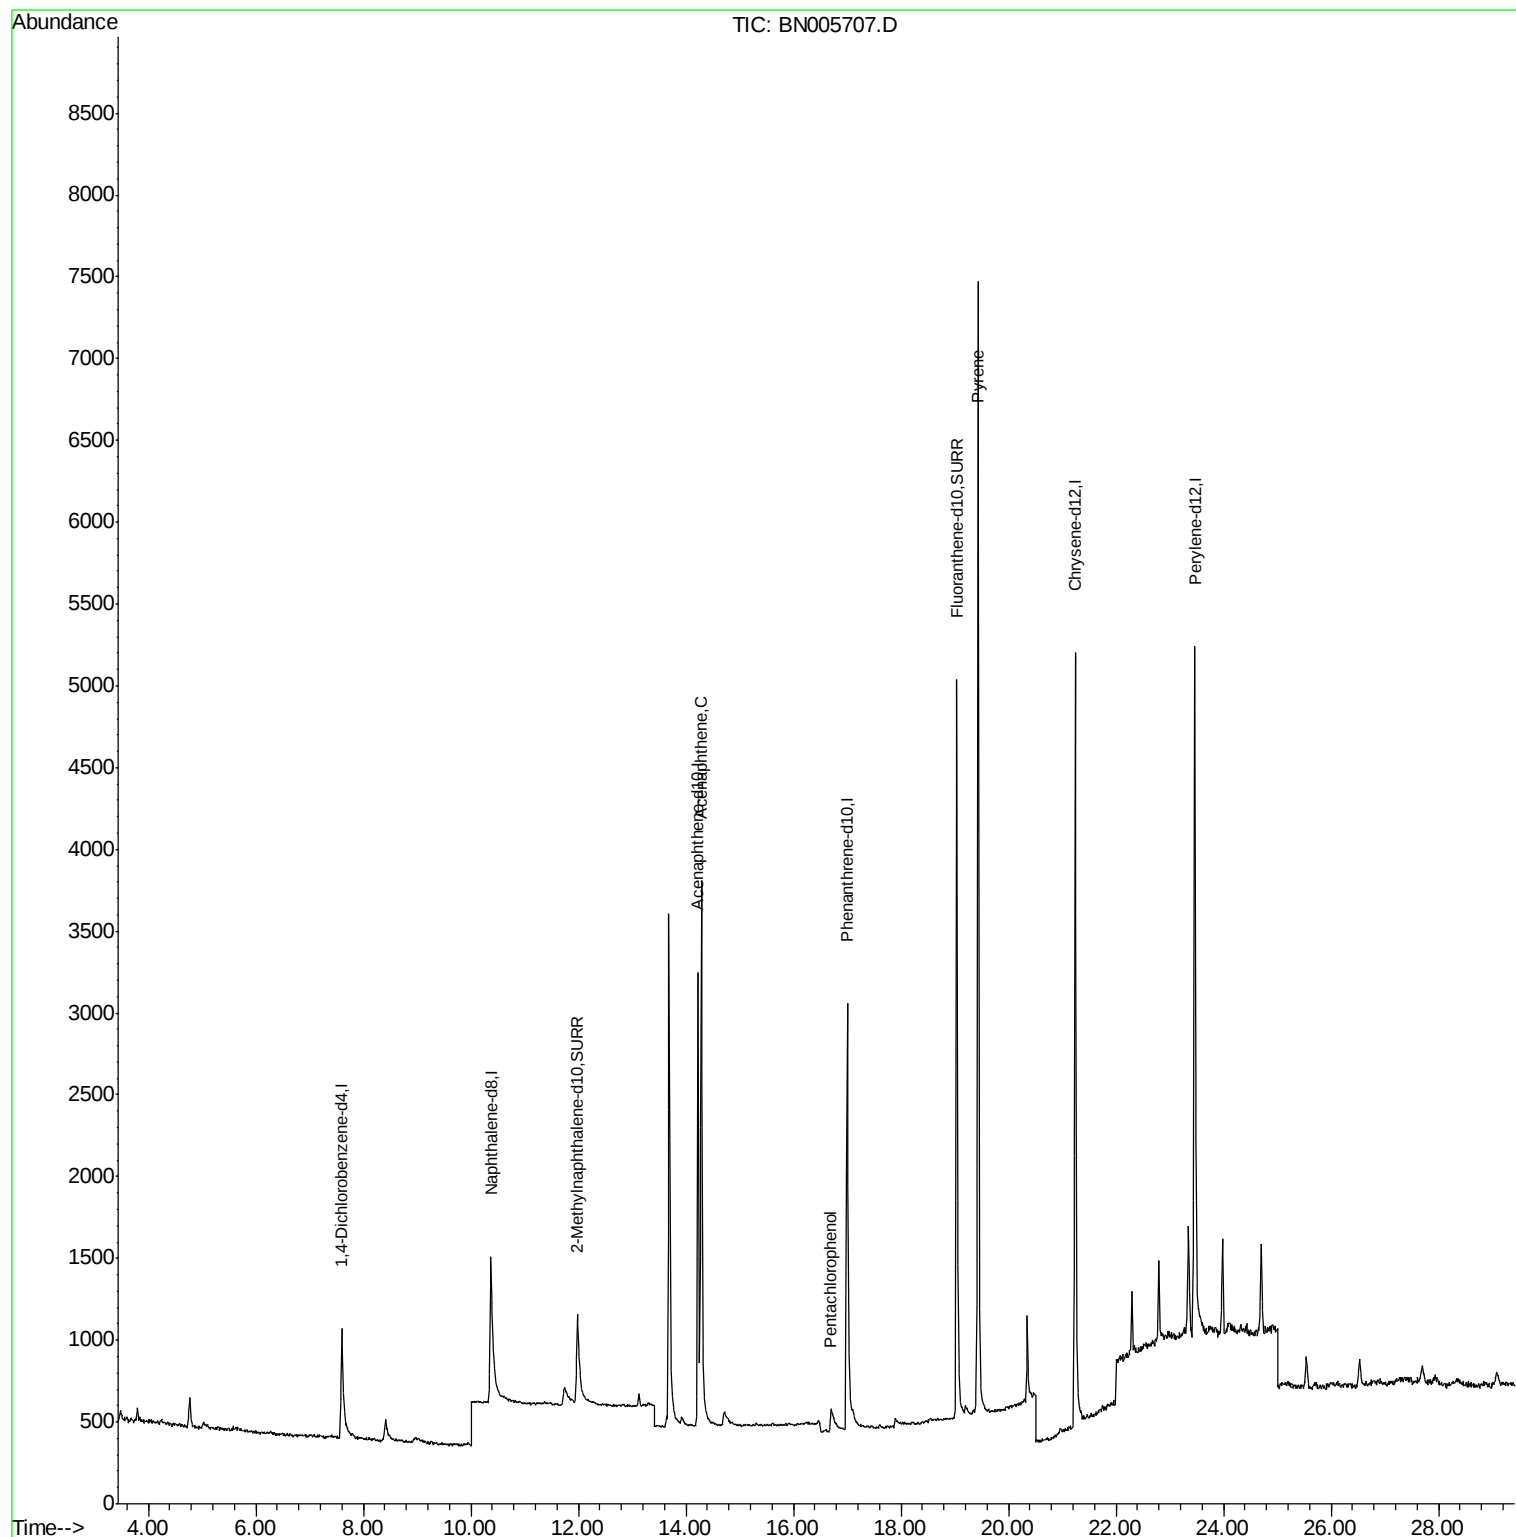

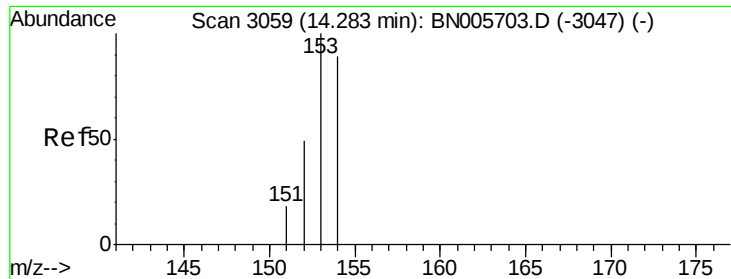

#8

Acenaphthene

Concen: 0.334 ng/ul

RT: 14.28 min Scan# 3059

Delta R.T. -0.01 min

Lab File: BN005707.D

Acq: 16 May 2019 17:25

Instrument :

BNA_N

ClientSampleId :

A5167MSD


Tot Ion:153 Resp: 2406

Ion Ratio Lower Upper




153 100

152 52.5 40.8 61.2

154 88.9 73.2 109.8

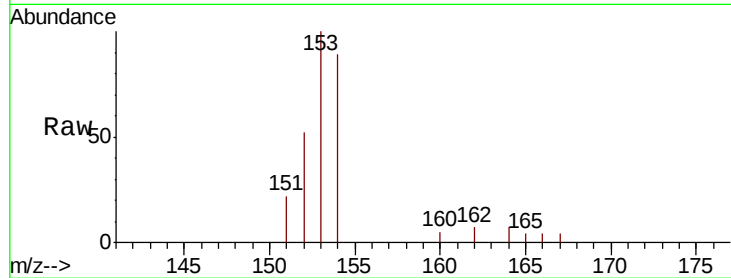

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

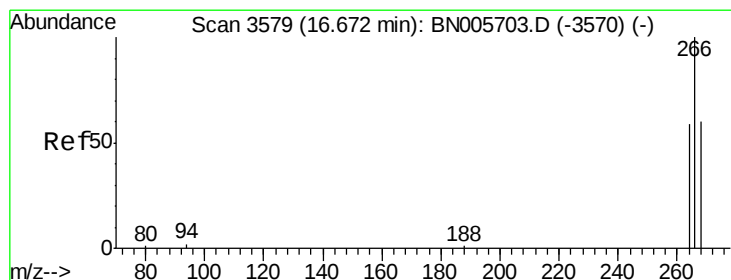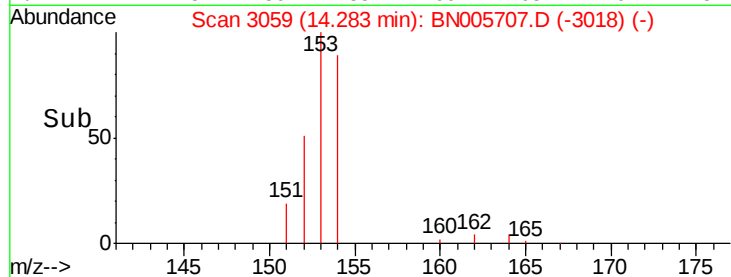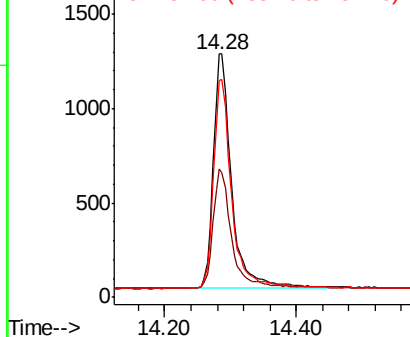

#11

Pentachlorophenol

Concen: 0.254 ng/ul

RT: 16.70 min Scan# 3586

Delta R.T. 0.00 min

Lab File: BN005707.D

Acq: 16 May 2019 17:25


Tgt Ion:266 Resp: 334

Ion Ratio Lower Upper



266 100


264 55.4 55.3 82.9

268 52.1 56.7 85.1#

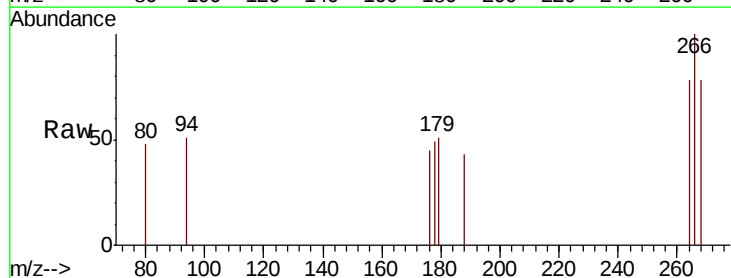

Abundance Ion 266.00 (265.70 to 266.70): E
Ion 264.00 (263.70 to 264.70): E
Ion 268.00 (267.70 to 268.70): E

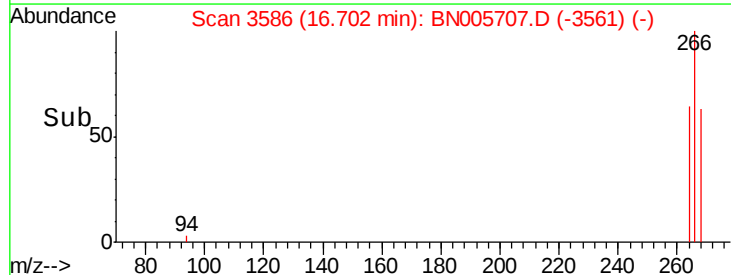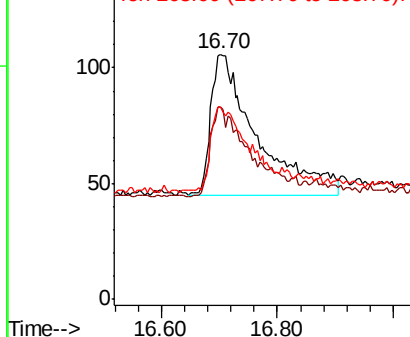

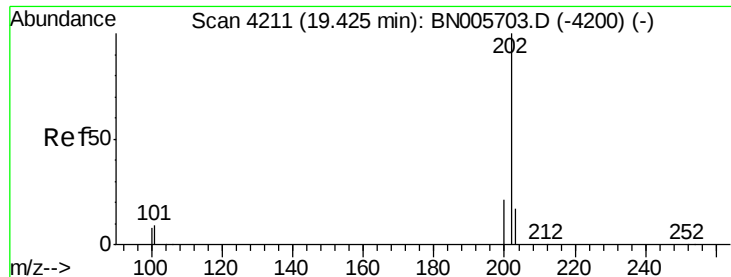

#17
 Pvrene
 Concen: 0.350 ng/ul
 RT: 19.43 min Scan# 4213
 Delta R.T. 0.00 min
 Lab File: BN005707.D
 Acq: 16 May 2019 17:25

Instrument :
 BNA_N
 ClientSampleId :
 A5167MSD

Tot Ion	Ratio	Lower	Upper
202	100		
101	9.4	8.5	12.7
100	7.7	6.9	10.3

