

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN051619\
 Data File : BN005721.D
 Acq On : 17 May 2019 02:04
 Operator : JU/SJ
 Sample : K2788-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51A0

Manual Integrations
 APPROVED

mohammad
 5/17/2019 3:36:23 PM

Quant Time: May 17 14:12:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN050719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 17 04:47:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	1141	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.35	136	4956	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.23	164	3367	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.98	188	8227m	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	5780m	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	6187	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.96	152	2771	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.03	212	8375m	0.32	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.03	178	2649	0.118	ng/ul	Ovalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN051619\
Data File : BN005721.D
Acq On : 17 May 2019 02:04
Operator : JU/SJ
Sample : K2788-11
Misc :
ALS Vial : 18 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
A51A0

Manual Integrations
APPROVED

mohammad
5/17/2019 3:36:23 PM

Quant Time: May 17 14:12:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 17 04:47:07 2019
Response via : Initial Calibration

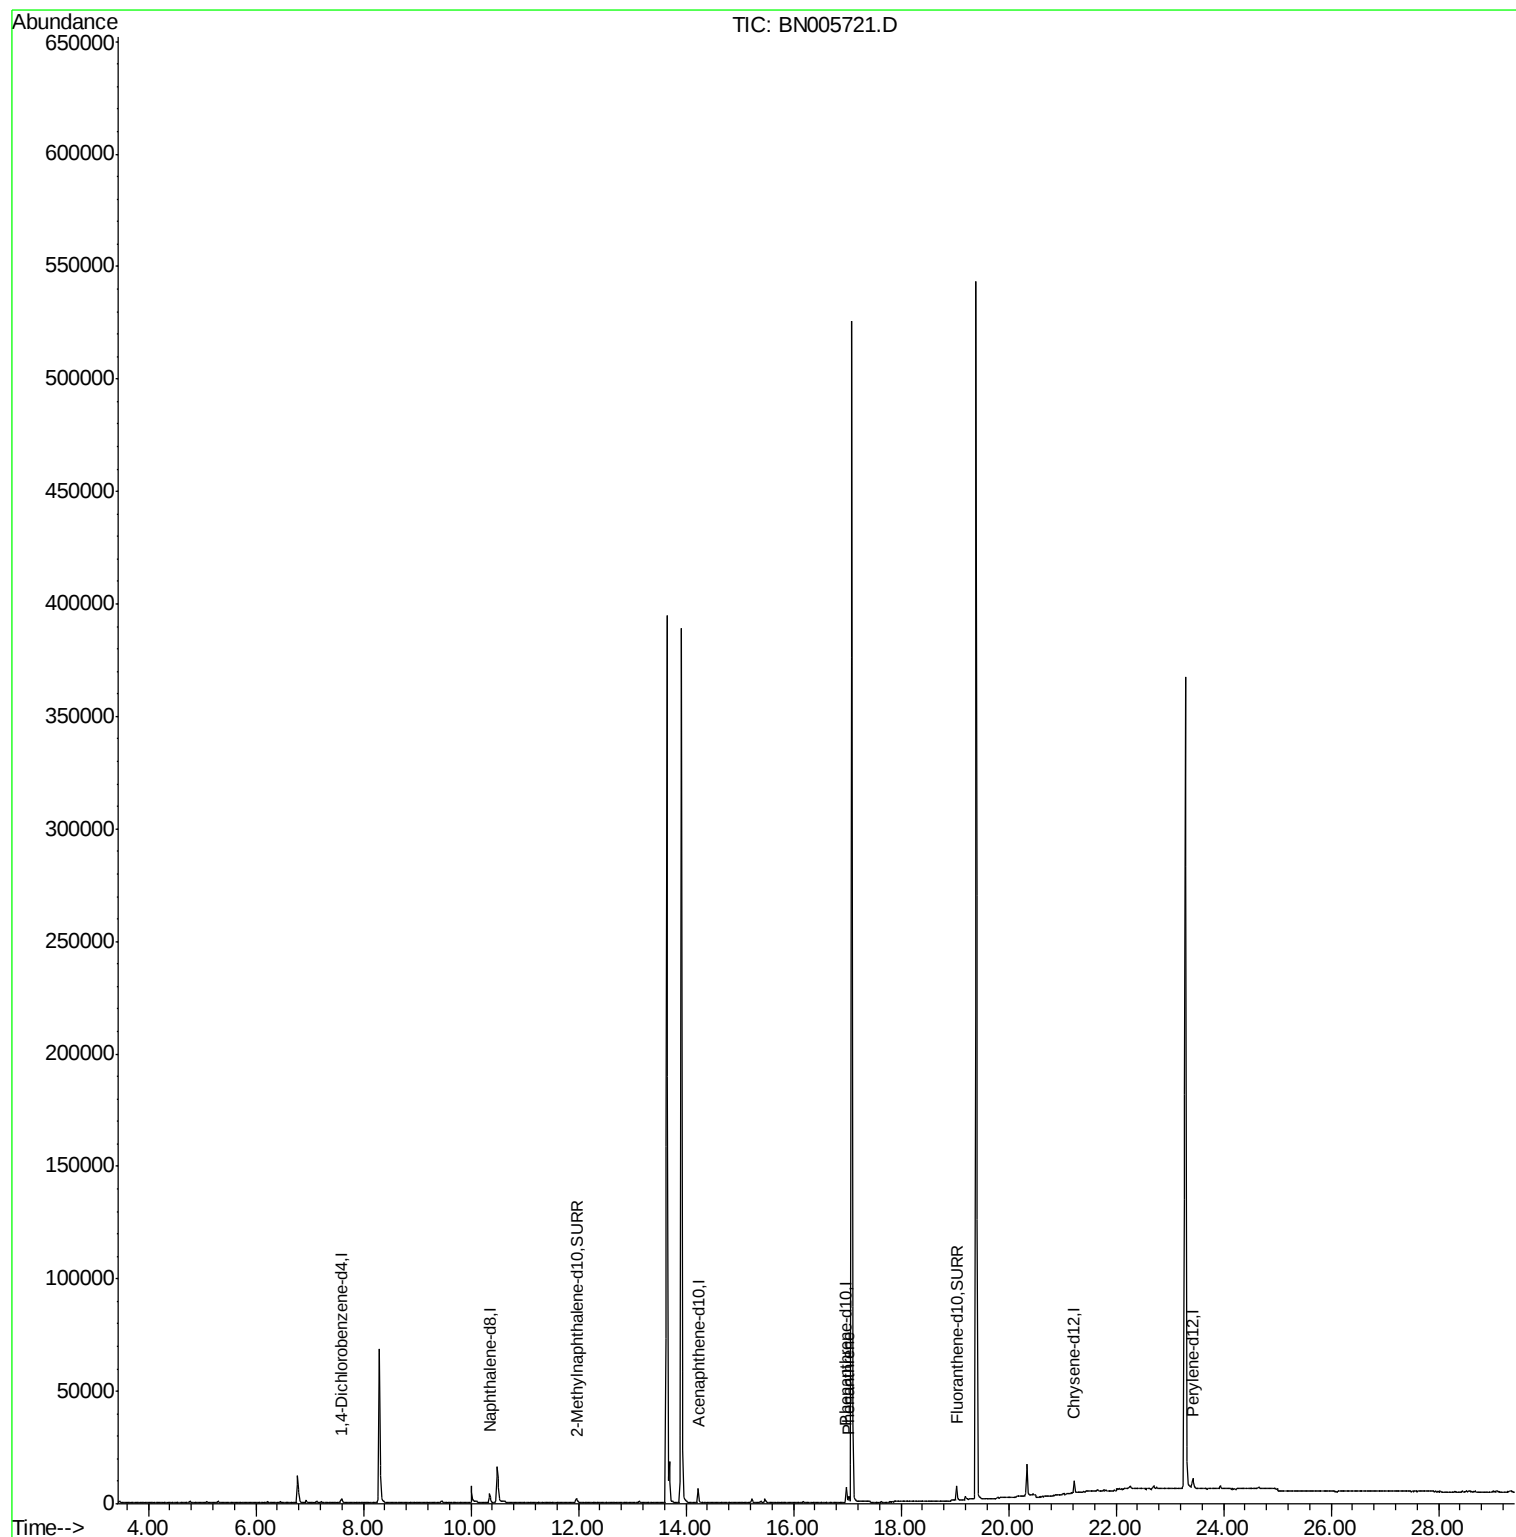

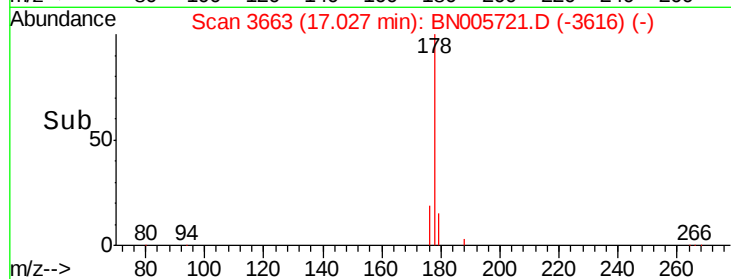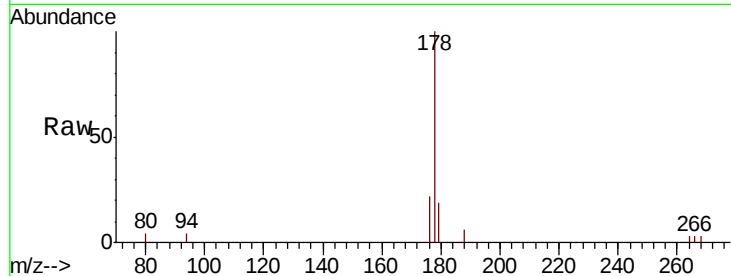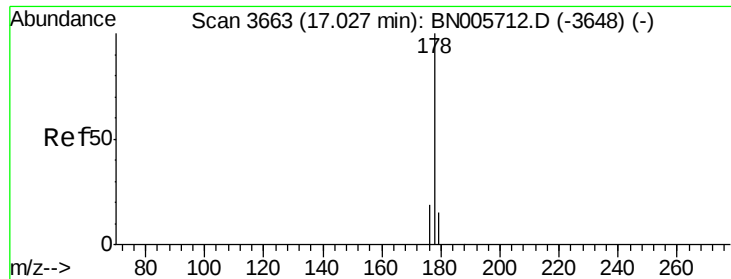

#12

Phenanthrene

Concen: 0.118 ng/ul

RT: 17.03 min Scan# 3663

Delta R.T. -0.00 min

Lab File: BN005721.D

Acq: 17 May 2019 02:04

Tot Ion:	178	Resp:	2649
Ion Ratio	Lower	Upper	
178	100		
179	19.1	12.8	19.2
176	22.0	15.3	22.9

Instrument :

BNA_N

ClientSampleId :

A51A0

Manual Integrations
APPROVED

mohammad
5/17/2019 3:36:23 PM

