

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019795.D
 Acq On : 16 May 2022 16:59
 Operator : CG/JU
 Sample : N2707-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXL89

Quant Time: May 17 01:43:18 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	3746	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136	12772	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.479	164	8043	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.217	188	17637	0.400	ng/ul	0.00
17) Chrysene-d12	21.406	240	16490	0.400	ng/ul	0.00
23) Perylene-d12	23.744	264	17218	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	20082	4.530	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152	7253	0.375	ng/ul	0.00
18) Fluoranthene-d10	19.244	212	19761	0.379	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.611	202	2603	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.598	252	5750	0.077	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
Data File : BN019795.D
Acq On : 16 May 2022 16:59
Operator : CG/JU
Sample : N2707-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXL89

Quant Time: May 17 01:43:18 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration




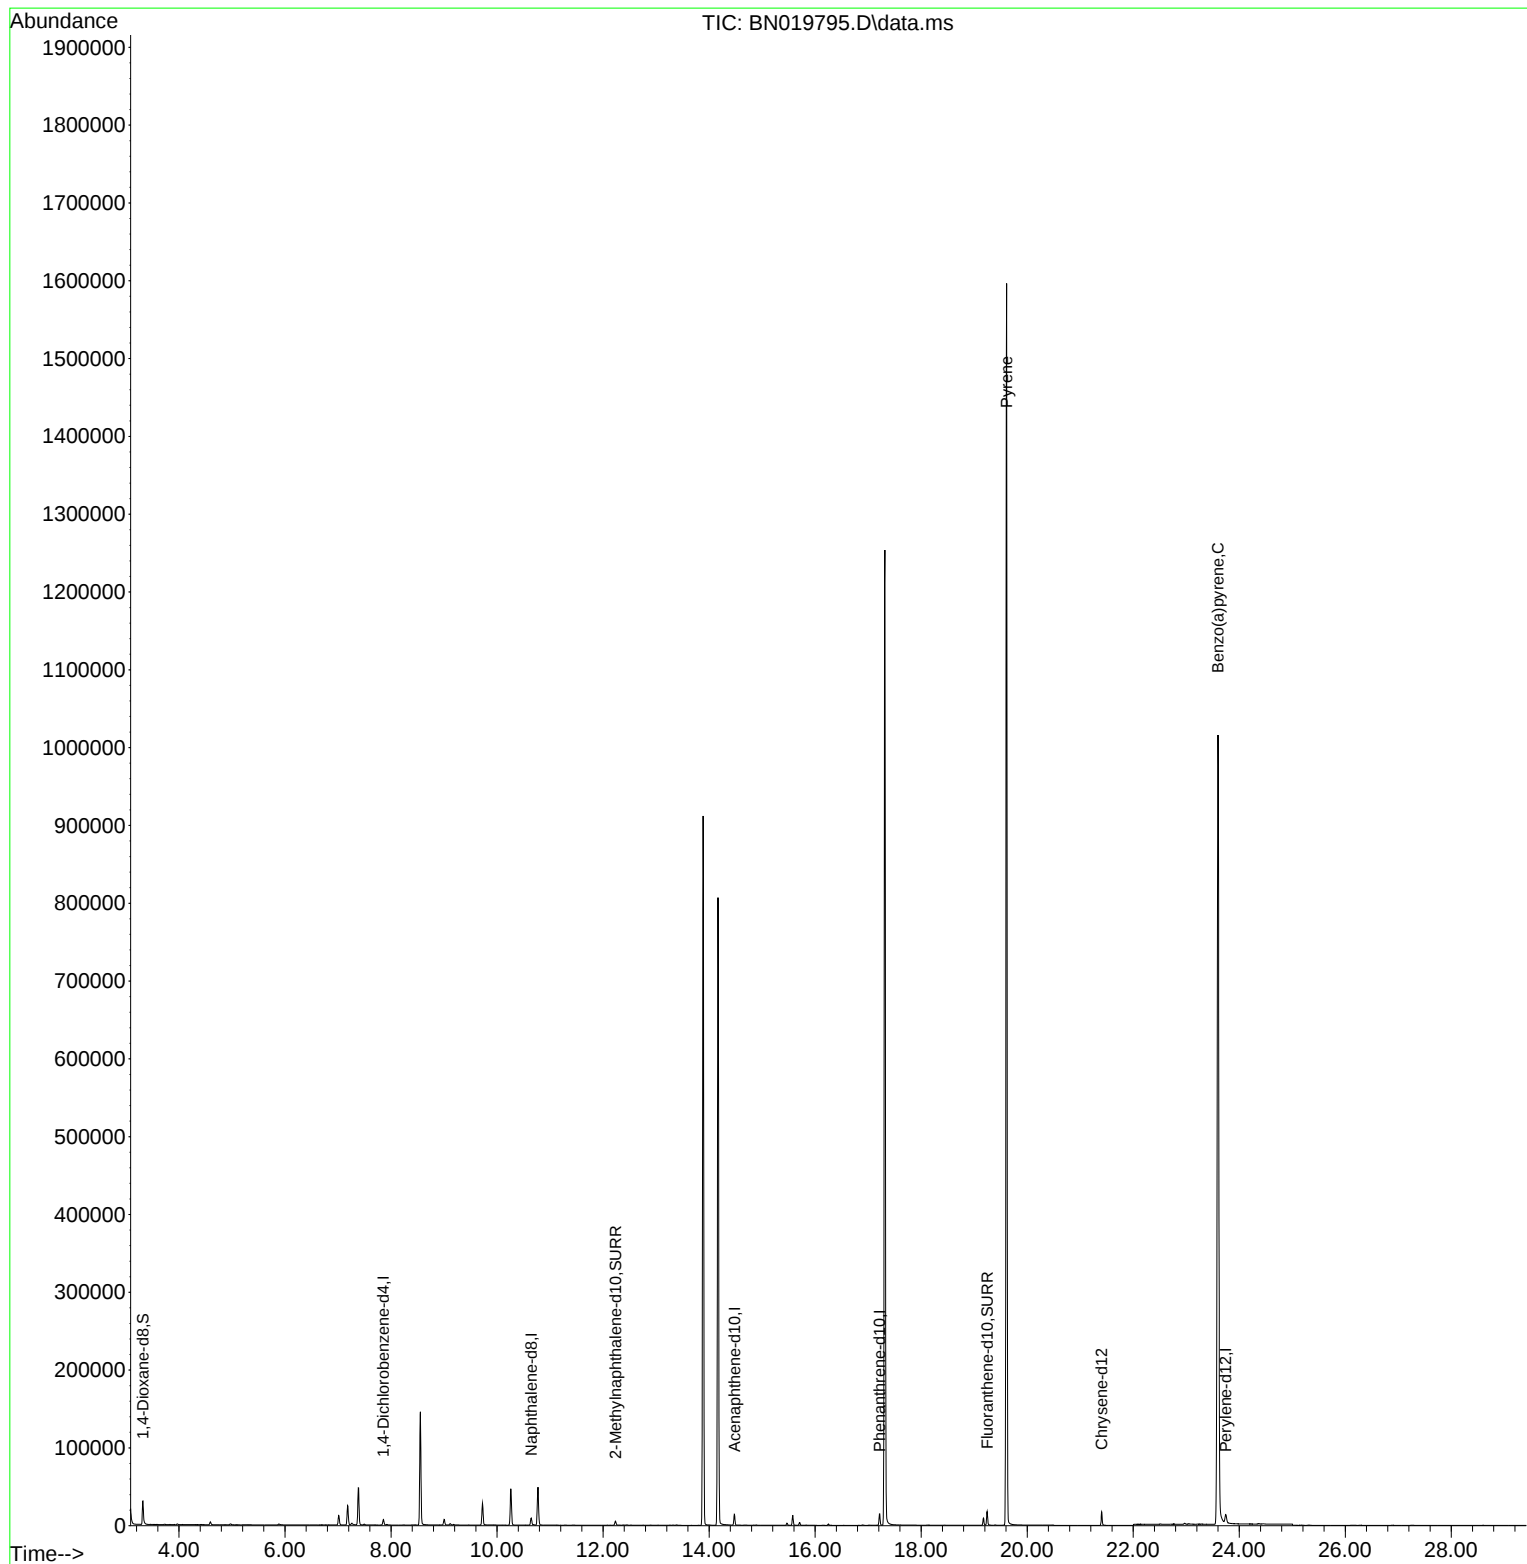


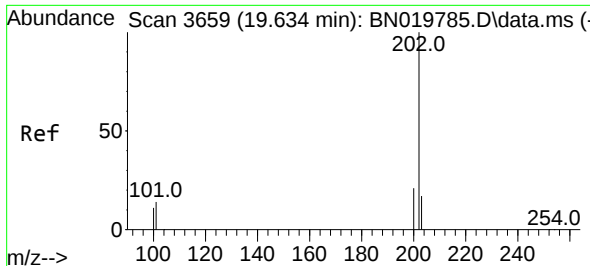

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.611 min Scan# 30
Delta R.T. -0.023 min
Lab File: BN019795.D
Acq: 16 May 2022 16:59

Instrument :
BNA_N
ClientSampleId :
EXL89

Tgt Ion:202 Resp: 2603
Ion Ratio Lower Upper
202 100
101 171.6 11.4 17.0#
100 1247.4 9.0 13.4#

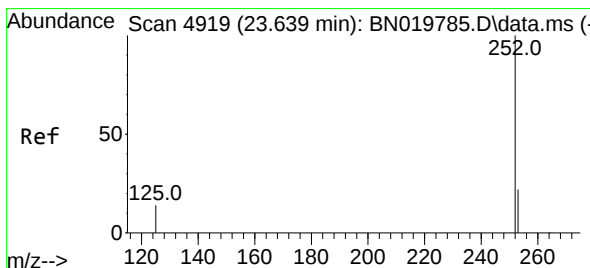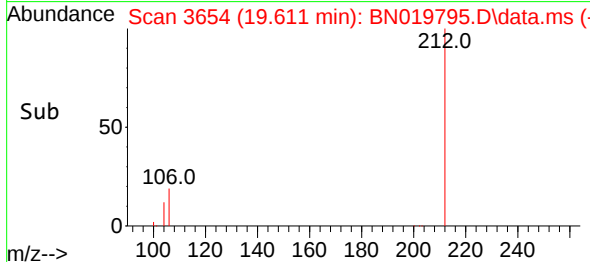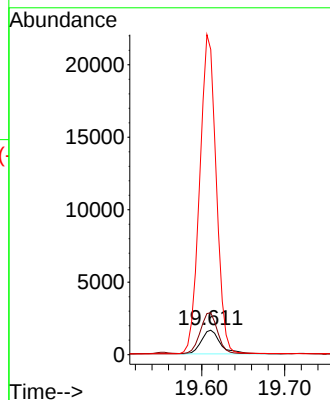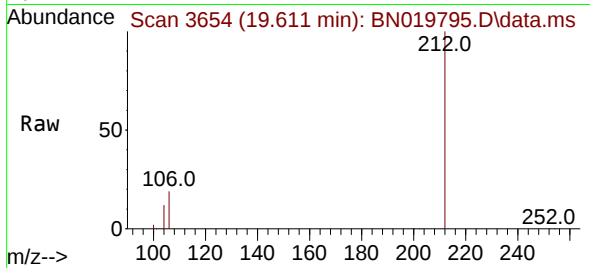

#26
Benzo(a)pyrene
Concen: 0.077 ng/ul
RT: 23.598 min Scan# 4905
Delta R.T. -0.041 min
Lab File: BN019795.D
Acq: 16 May 2022 16:59

Tgt Ion:252 Resp: 5750
Ion Ratio Lower Upper
252 100
253 39.0 23.4 35.0#
125 35.4 28.3 42.5

