

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019797.D
 Acq On : 16 May 2022 18:12
 Operator : CG/JU
 Sample : N2707-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXLA1

Quant Time: May 17 01:43:24 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	4166	0.400	ng/ul	0.00
4) Naphthalene-d8	10.643	136	14159	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.477	164	8921	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.216	188	19222	0.400	ng/ul	0.00
17) Chrysene-d12	21.403	240	17340	0.400	ng/ul	0.00
23) Perylene-d12	23.738	264	18790	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	21059	4.271	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.233	152	8368	0.391	ng/ul	0.00
18) Fluoranthene-d10	19.242	212	21731	0.396	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.609	202	2807	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.592	252	6434	0.079	ng/ul#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
Data File : BN019797.D
Acq On : 16 May 2022 18:12
Operator : CG/JU
Sample : N2707-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXLA1

Quant Time: May 17 01:43:24 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

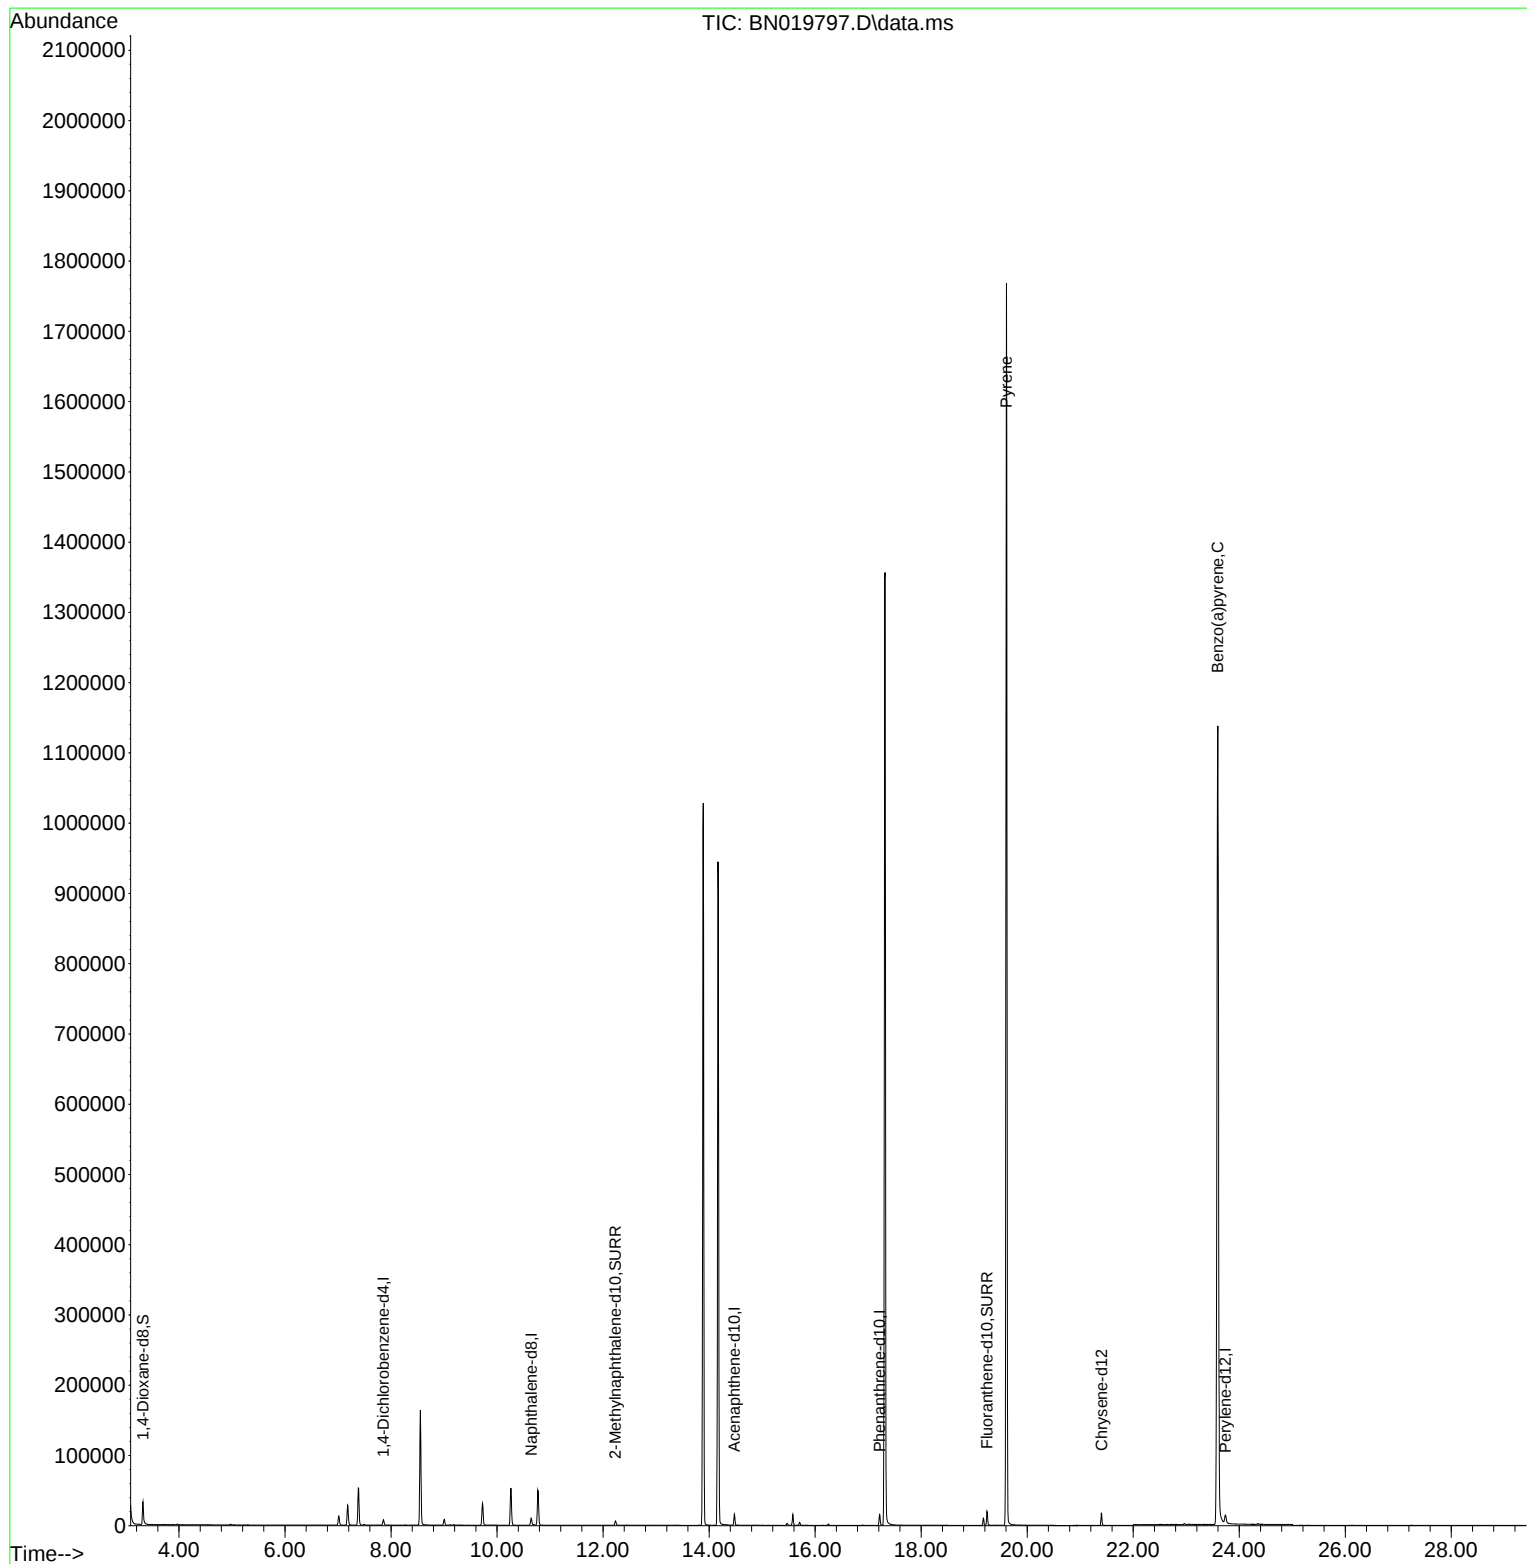

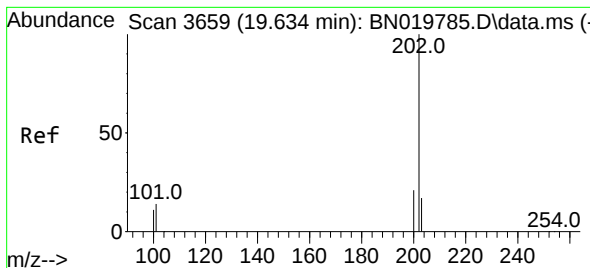

#20

Pyrene

Concen: 0.035 ng/ul

RT: 19.609 min Scan# 30

Delta R.T. -0.025 min

Lab File: BN019797.D

Acq: 16 May 2022 18:12

Instrument :

BNA_N

ClientSampleId :

EXLA1





Tgt Ion:202 Resp: 2807

Ion Ratio Lower Upper

202 100

101 174.0 11.4 17.0#

100 1283.5 9.0 13.4#

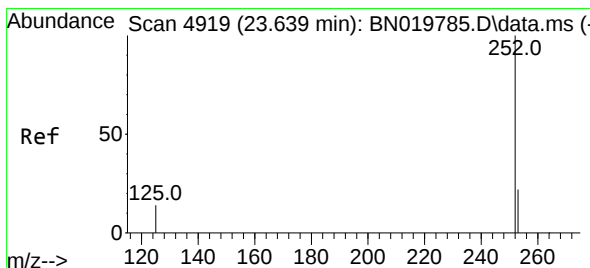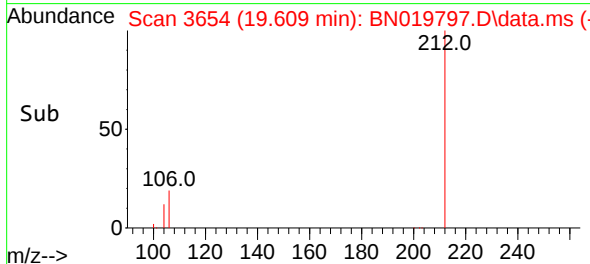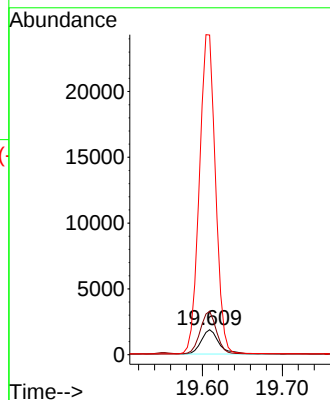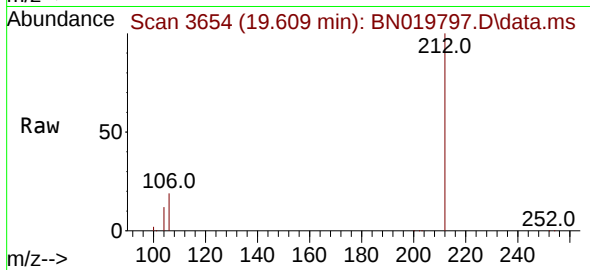

#26

Benzo(a)pyrene

Concen: 0.079 ng/ul

RT: 23.592 min Scan# 4903

Delta R.T. -0.047 min

Lab File: BN019797.D

Acq: 16 May 2022 18:12

Tgt Ion:252 Resp: 6434

Ion Ratio Lower Upper

252 100

253 37.0 23.4 35.0#

125 32.3 28.3 42.5

