

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019801.D
 Acq On : 16 May 2022 21:14
 Operator : CG/JU
 Sample : PB144801BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK801

Quant Time: May 17 01:43:37 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	3839	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136	13235	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.475	164	8443	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.214	188	17926	0.400	ng/ul	0.00
17) Chrysene-d12	21.400	240	15281	0.400	ng/ul	0.00
23) Perylene-d12	23.742	264	16201	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	30845	6.789	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152	7855	0.392	ng/ul	0.00
18) Fluoranthene-d10	19.244	212	17934	0.371	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.607	202	2334	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.593	252	5482	0.078	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
Data File : BN019801.D
Acq On : 16 May 2022 21:14
Operator : CG/JU
Sample : PB144801BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK801

Quant Time: May 17 01:43:37 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration




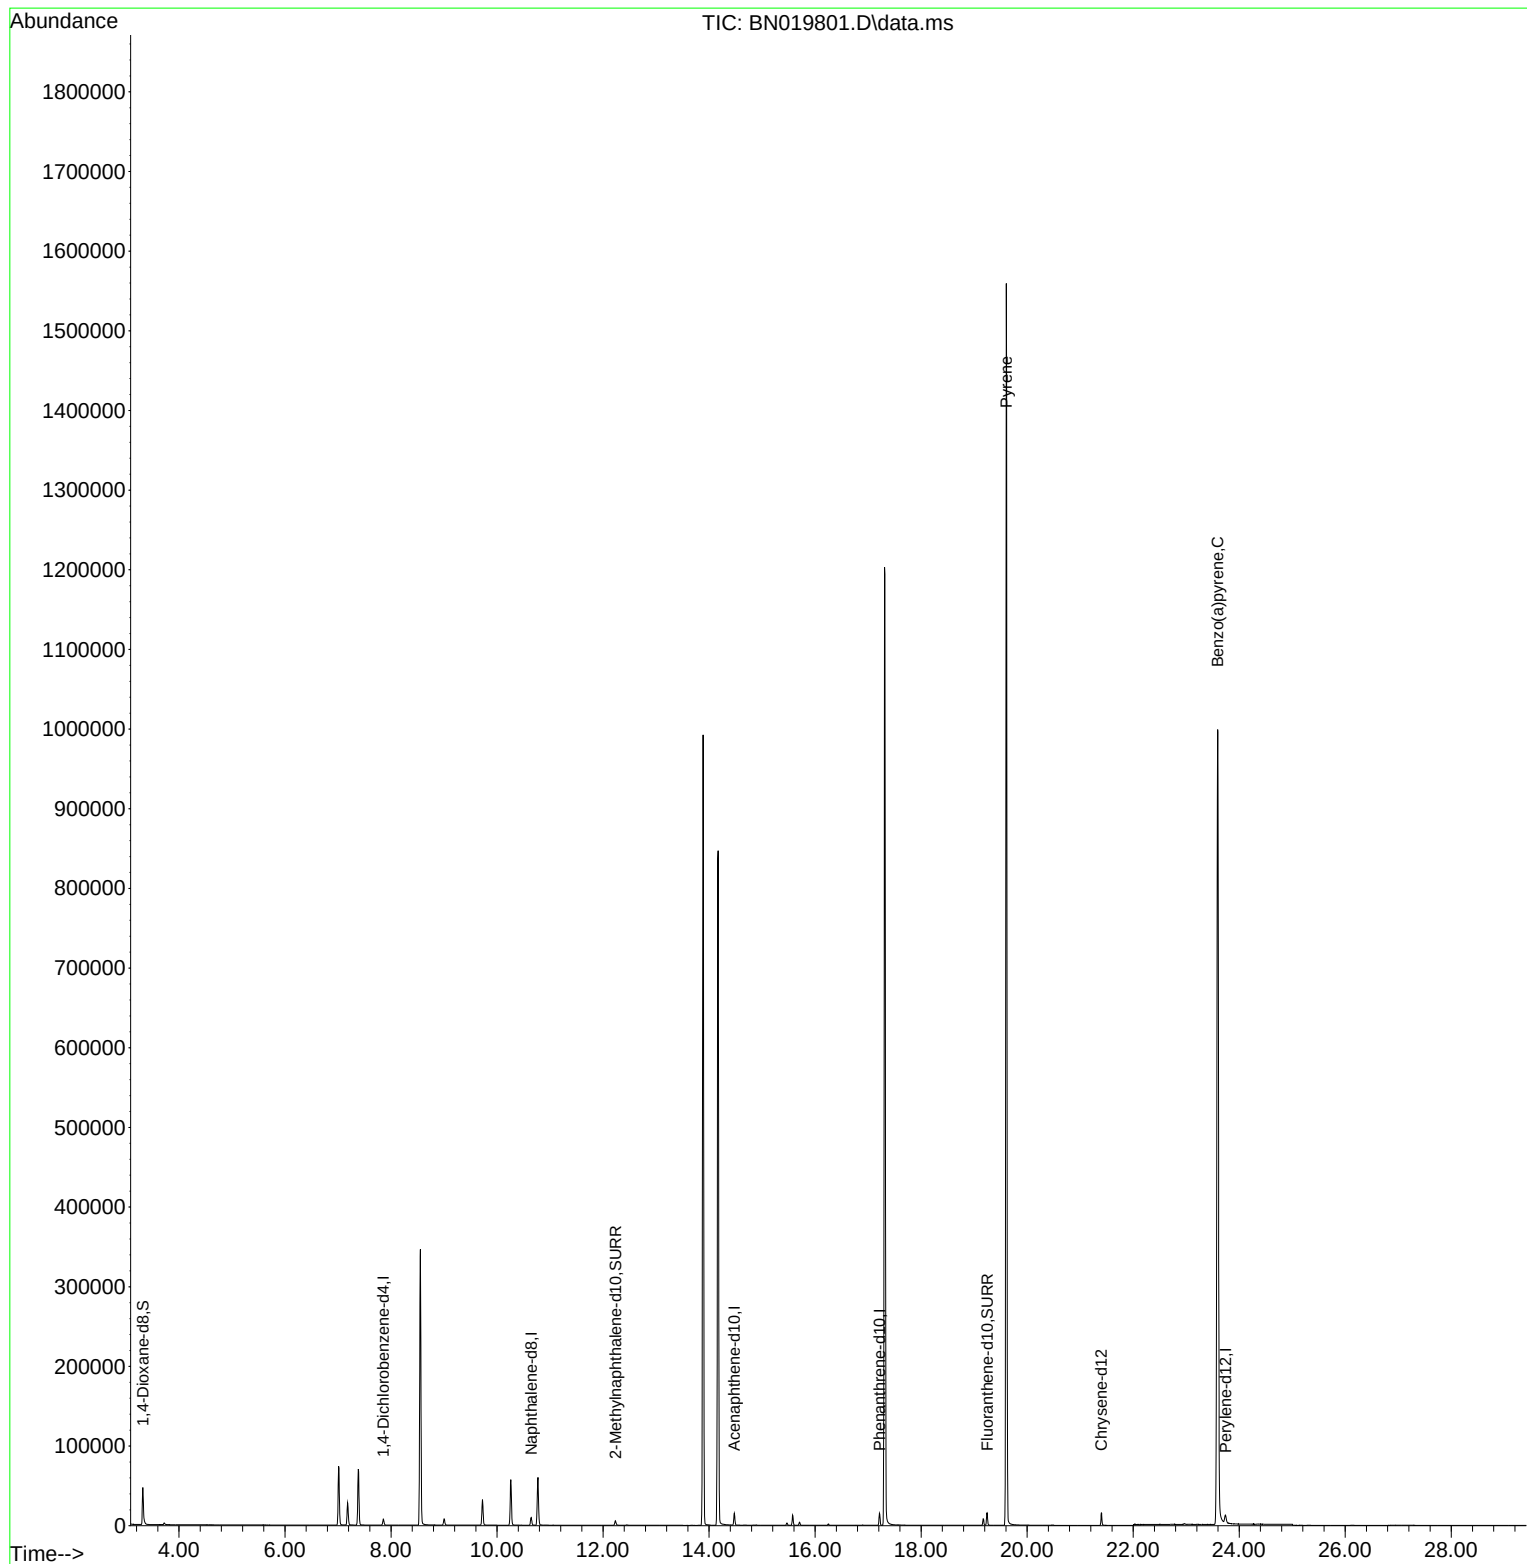


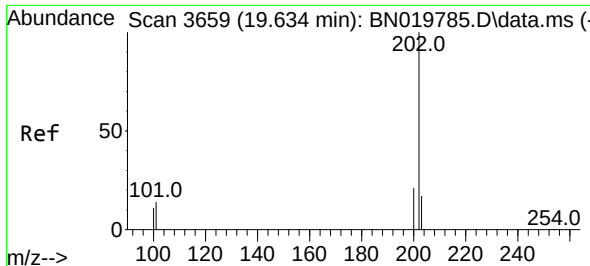

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.607 min Scan# 3653
Delta R.T. -0.027 min
Lab File: BN019801.D
Acq: 16 May 2022 21:14

Instrument :
BNA_N
ClientSampleId :
SBLK801

Tgt Ion:202 Resp: 2334
Ion Ratio Lower Upper
202 100
101 174.5 11.4 17.0#
100 1308.1 9.0 13.4#

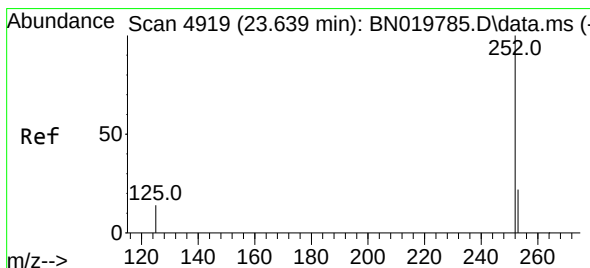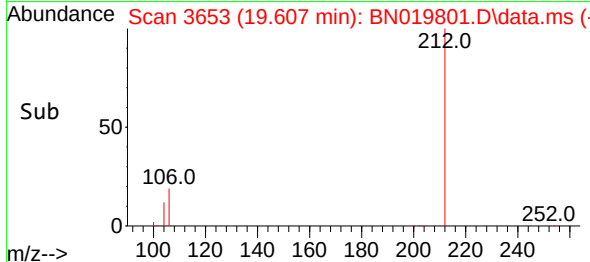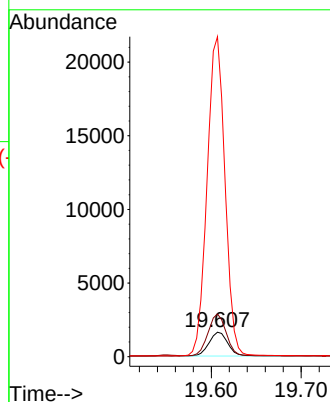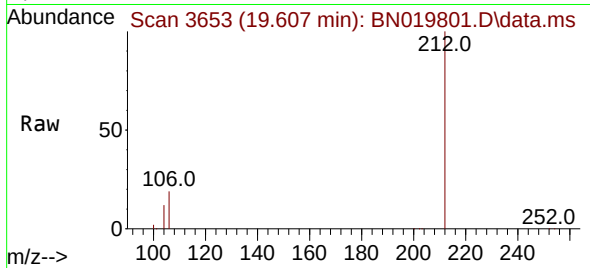

#26
Benzo(a)pyrene
Concen: 0.078 ng/ul
RT: 23.593 min Scan# 4903
Delta R.T. -0.046 min
Lab File: BN019801.D
Acq: 16 May 2022 21:14

Tgt Ion:252 Resp: 5482
Ion Ratio Lower Upper
252 100
253 38.0 23.4 35.0#
125 32.4 28.3 42.5

