




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019786.D
 Acq On : 16 May 2022 11:31
 Operator : CG/JU
 Sample : PB144621BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK621

Manual IntegrationsAPPROVED

Quant Time: May 17 01:42:39 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

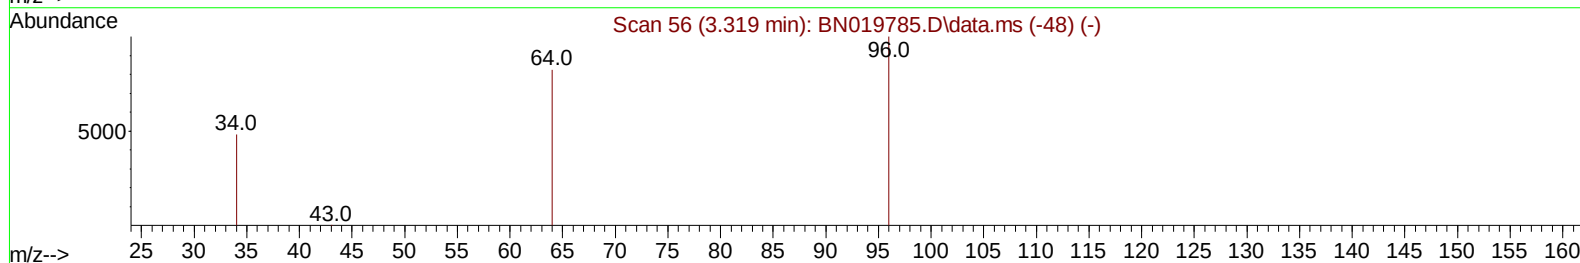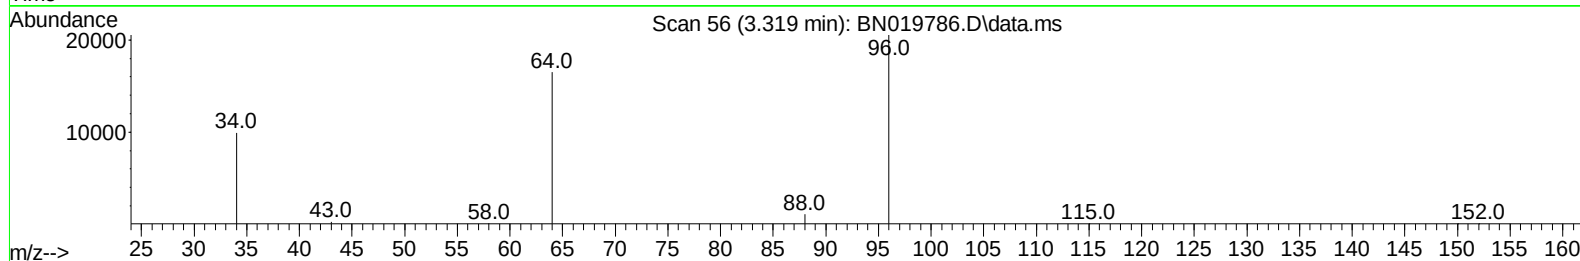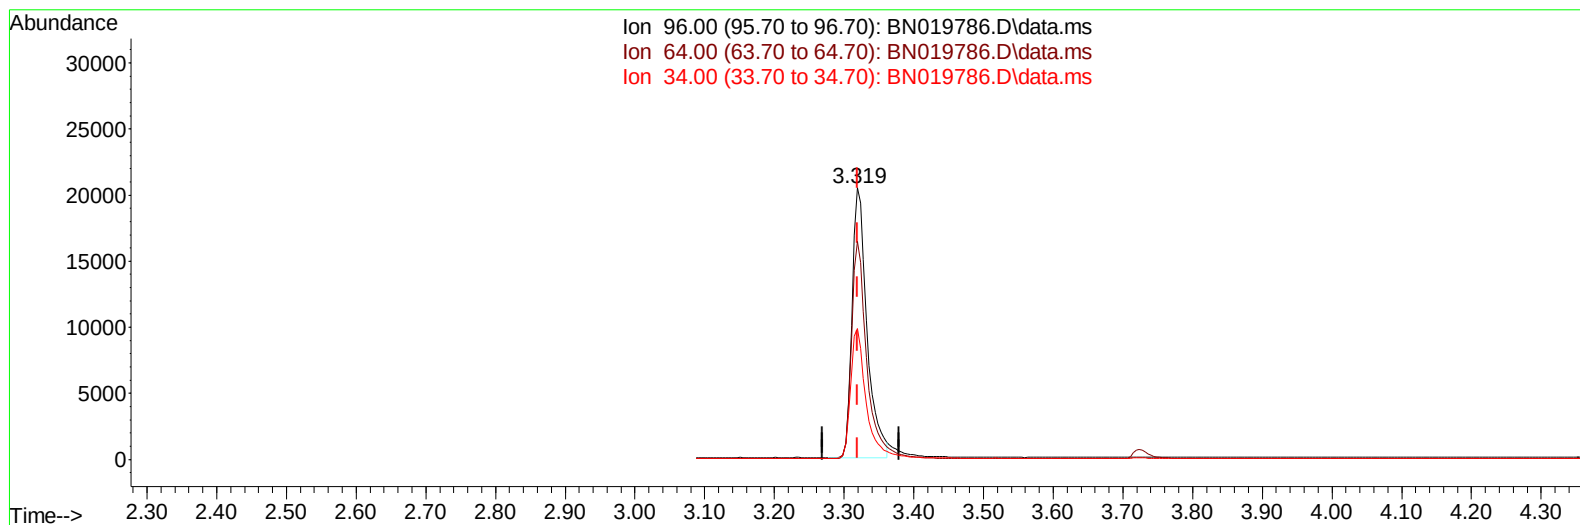

TIC: BN019786.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 5.79 ng/u1

response 30268

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	80.26#
34.00	22.70	48.15#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019786.D
 Acq On : 16 May 2022 11:31
 Operator : CG/JU
 Sample : PB144621BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK621

Manual IntegrationsAPPROVED

Quant Time: May 17 01:42:39 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

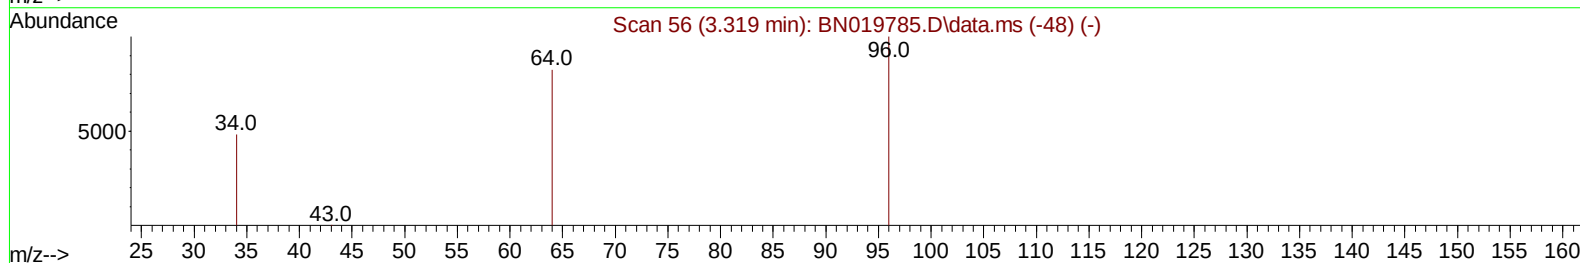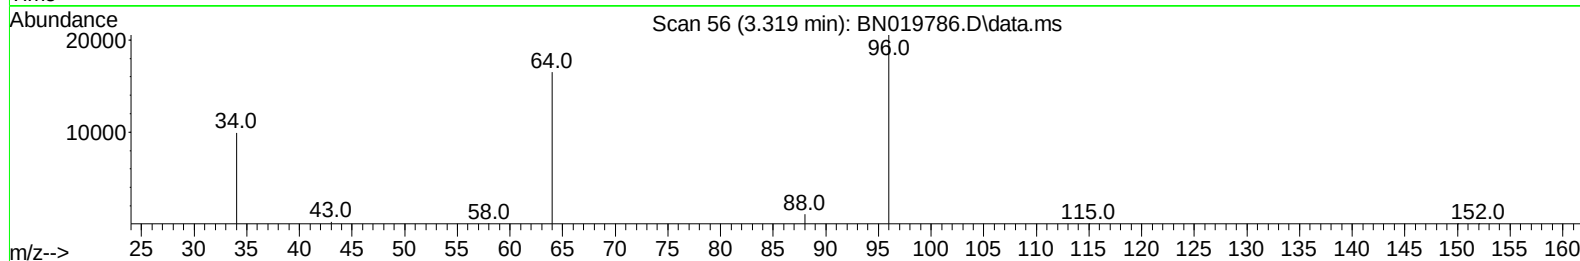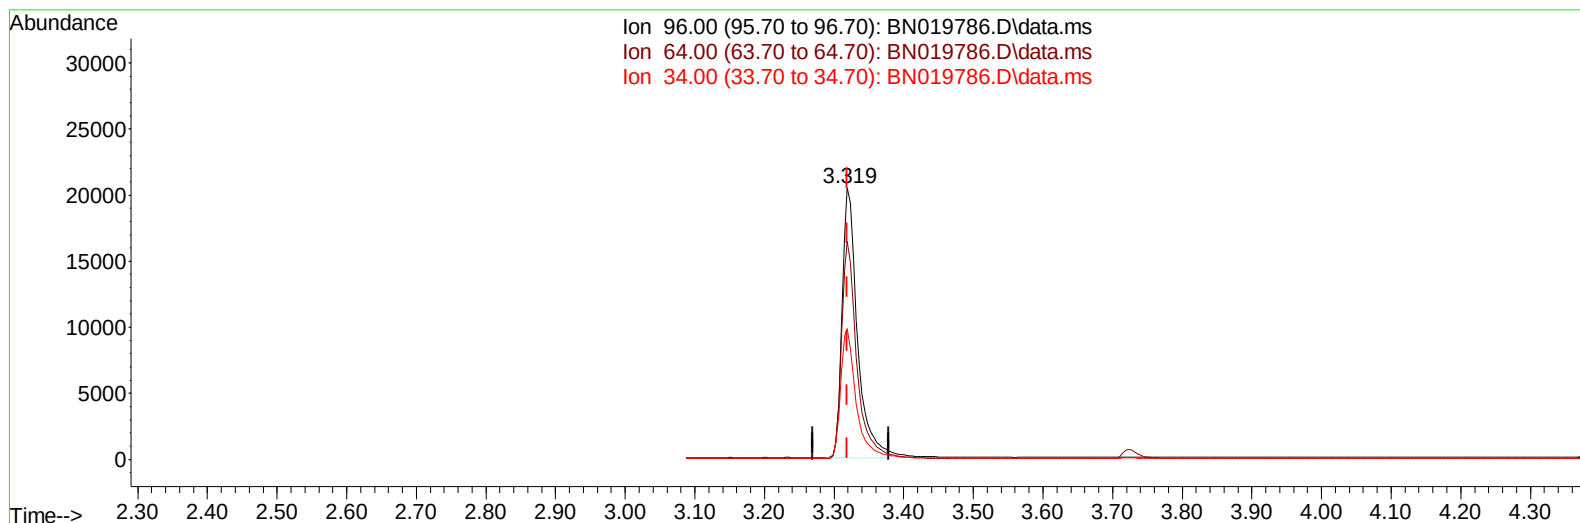

TIC: BN019786.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 5.93 ng/ul m

response 31003

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	80.26#
34.00	22.70	48.15#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019786.D
 Acq On : 16 May 2022 11:31
 Operator : CG/JU
 Sample : PB144621BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK621

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 01:42:39 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.855	152		4418	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136		14755	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.475	164		9080	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.214	188		19284	0.400	ng/ul	0.00
17) Chrysene-d12	21.406	240		16164	0.400	ng/ul	0.00
23) Perylene-d12	23.745	264		18054	0.400	ng/ul #	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.319	96		31003m	5.929	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152		7266	0.325	ng/ul	0.00
18) Fluoranthene-d10	19.244	212		16101	0.315	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
Data File : BN019786.D
Acq On : 16 May 2022 11:31
Operator : CG/JU
Sample : PB144621BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK621

Manual IntegrationsAPPROVED

Quant Time: May 17 01:42:39 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022

