




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019791.D
 Acq On : 16 May 2022 14:32
 Operator : CG/JU
 Sample : N2707-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXL83

Manual IntegrationsAPPROVED

Quant Time: May 17 01:43:06 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

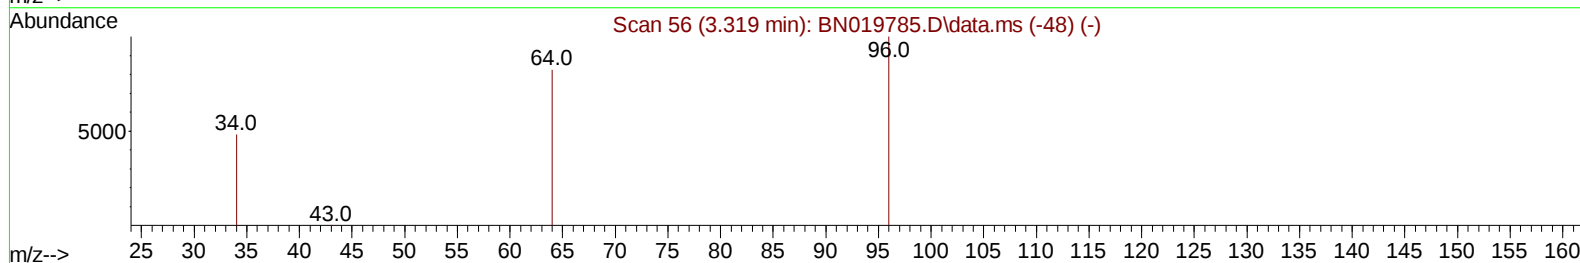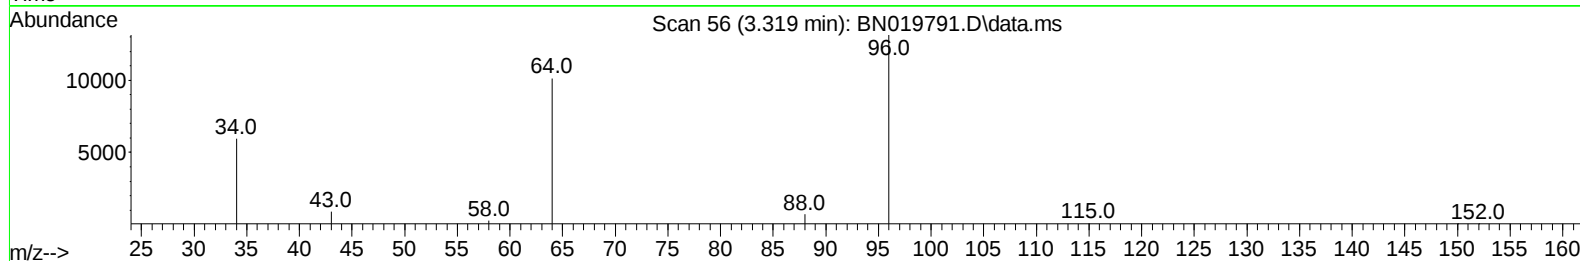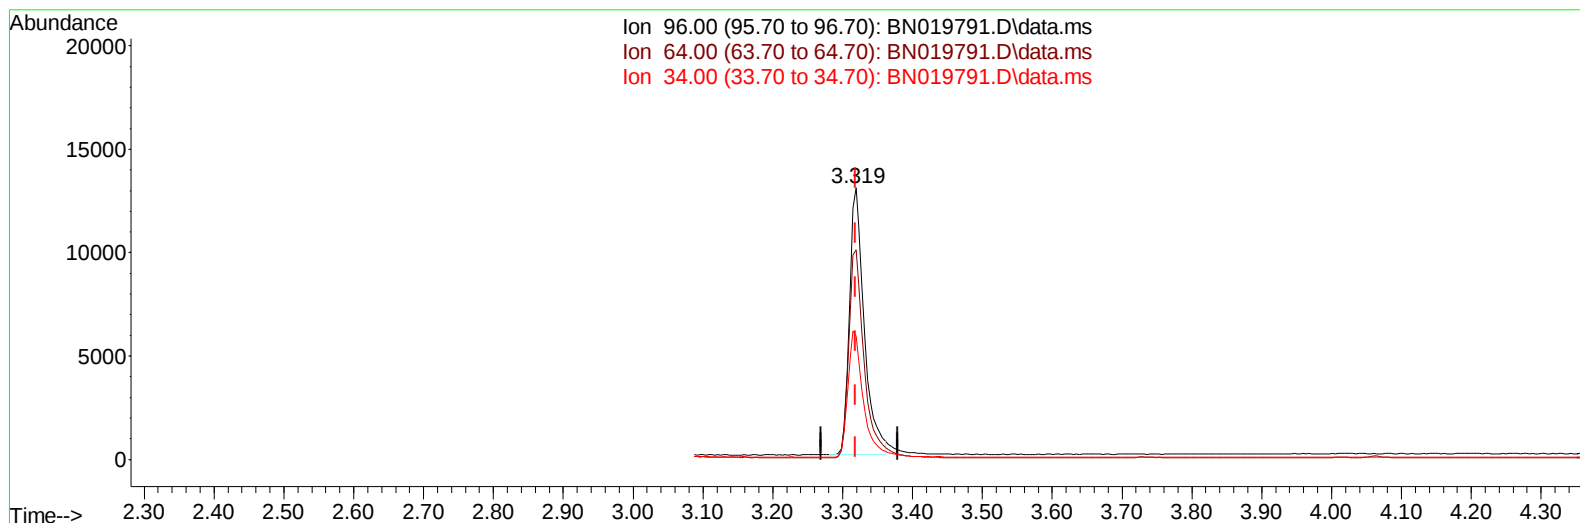

TIC: BN019791.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 4.34 ng/u1

response 18982

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	77.16#
34.00	22.70	45.48#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019791.D
 Acq On : 16 May 2022 14:32
 Operator : CG/JU
 Sample : N2707-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXL83

Manual IntegrationsAPPROVED

Quant Time: May 17 01:43:06 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

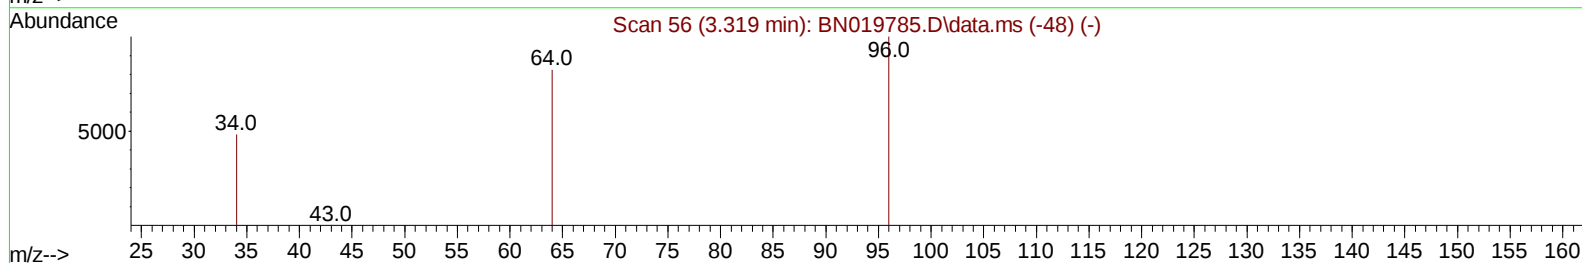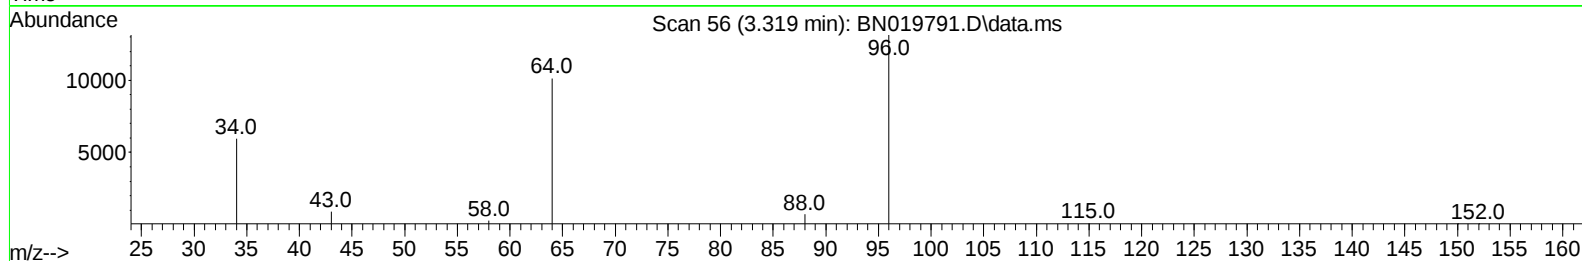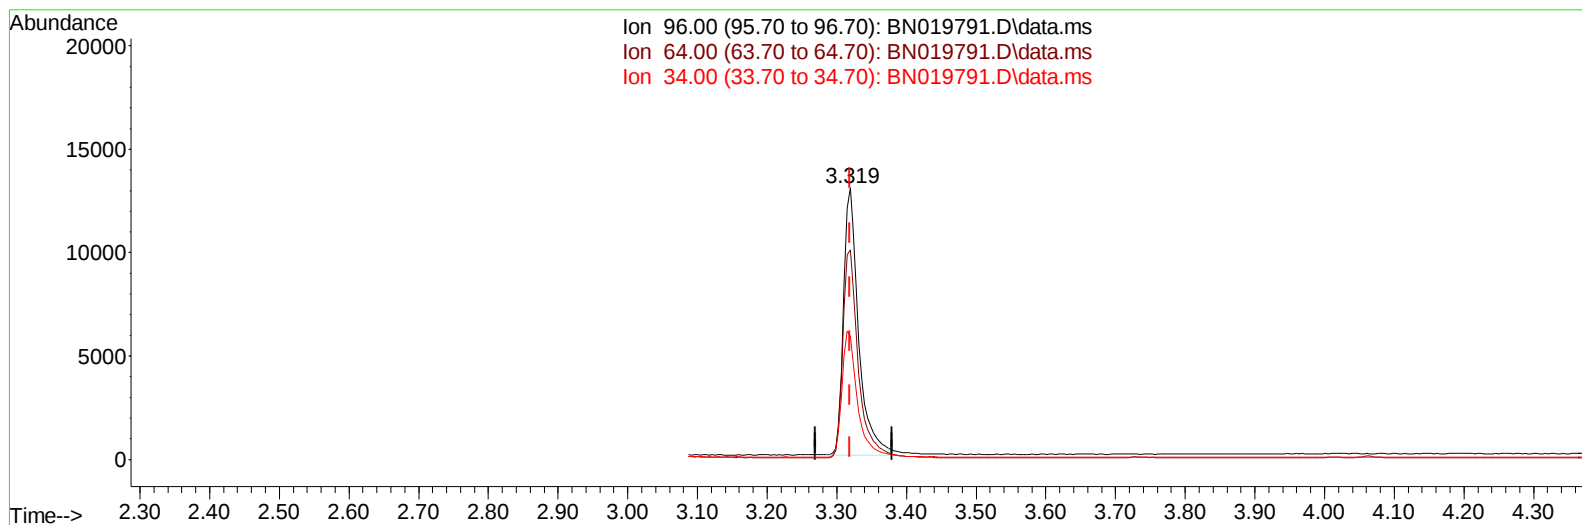

TIC: BN019791.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 4.44 ng/ul m

response 19387

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	77.16#
34.00	22.70	45.48#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019791.D
 Acq On : 16 May 2022 14:32
 Operator : CG/JU
 Sample : N2707-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXL83

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 01:43:06 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.855	152		3693	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136		12557	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.479	164		8165	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188		18779	0.400	ng/ul	0.00
17) Chrysene-d12	21.404	240		17761	0.400	ng/ul	0.00
23) Perylene-d12	23.745	264		17677	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.319	96		19387m	4.436	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152		6779	0.357	ng/ul	0.00
18) Fluoranthene-d10	19.253	212		21625	0.385	ng/ul	0.00
Target Compounds							
							Qvalue
5) Naphthalene	10.694	128		823	0.020	ng/ul#	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
Data File : BN019791.D
Acq On : 16 May 2022 14:32
Operator : CG/JU
Sample : N2707-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXL83

Manual IntegrationsAPPROVED

Quant Time: May 17 01:43:06 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022

