




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019798.D
 Acq On : 16 May 2022 18:48
 Operator : CG/JU
 Sample : N2707-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXL99

Manual IntegrationsAPPROVED

Quant Time: May 17 01:43:27 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

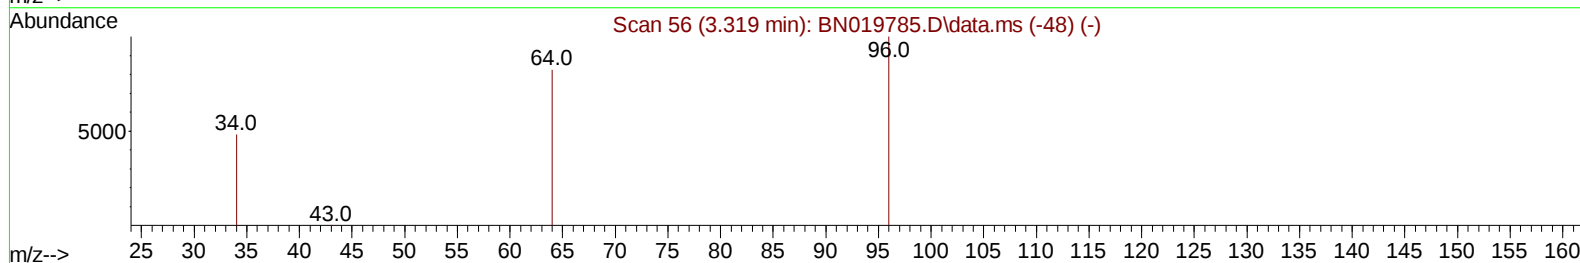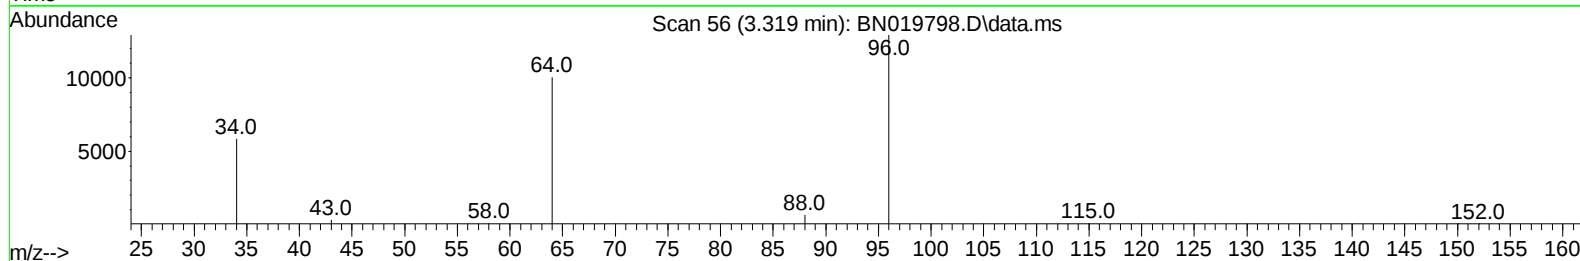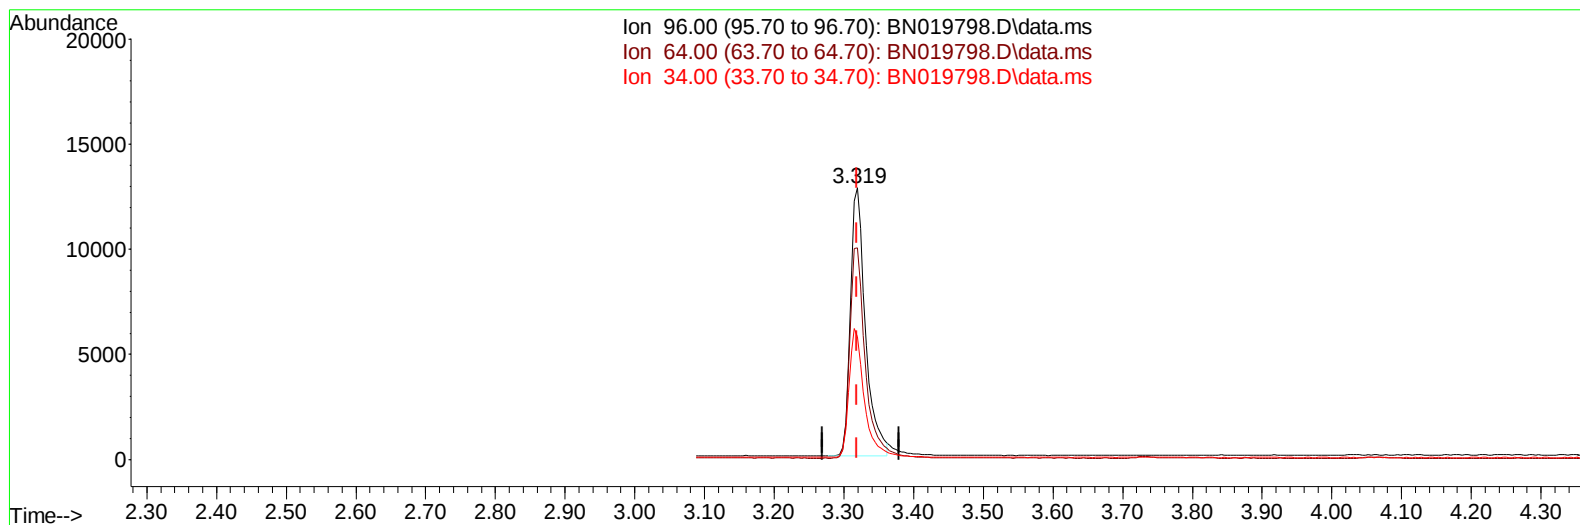

TIC: BN019798.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (+ 0.000) 3.74 ng/u1

response 19079

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	77.84#
34.00	22.70	45.26#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019798.D
 Acq On : 16 May 2022 18:48
 Operator : CG/JU
 Sample : N2707-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXL99

Manual IntegrationsAPPROVED

Quant Time: May 17 01:43:27 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

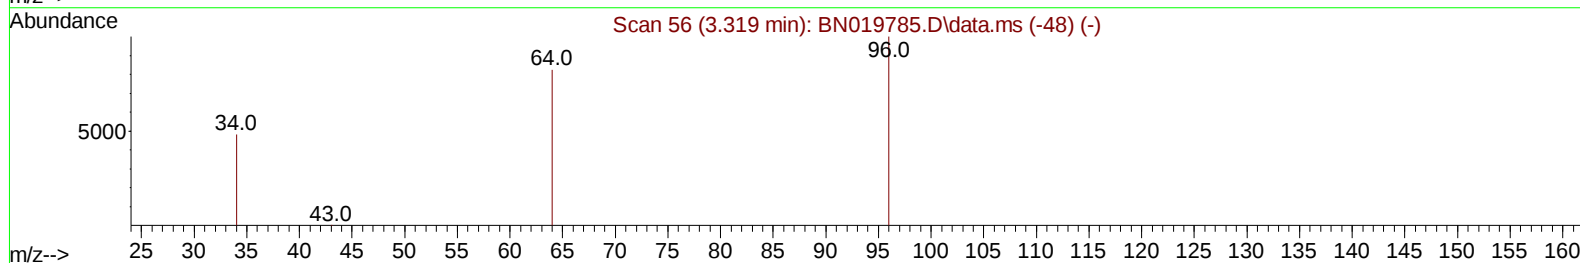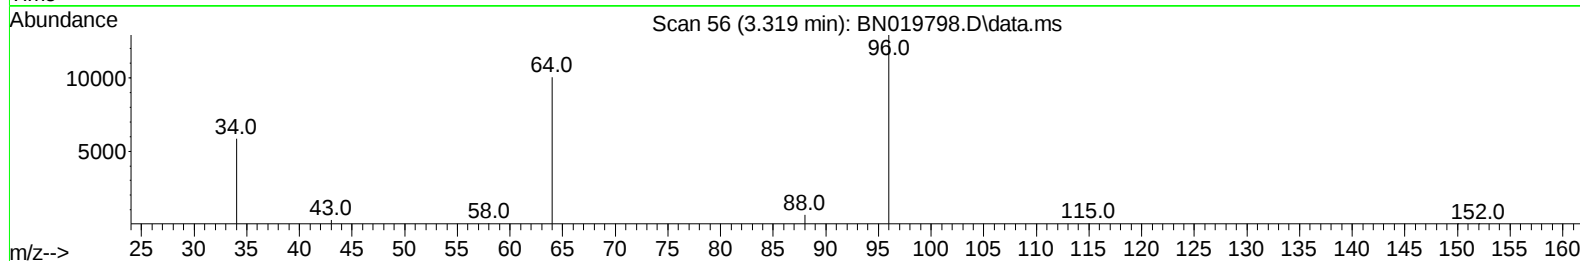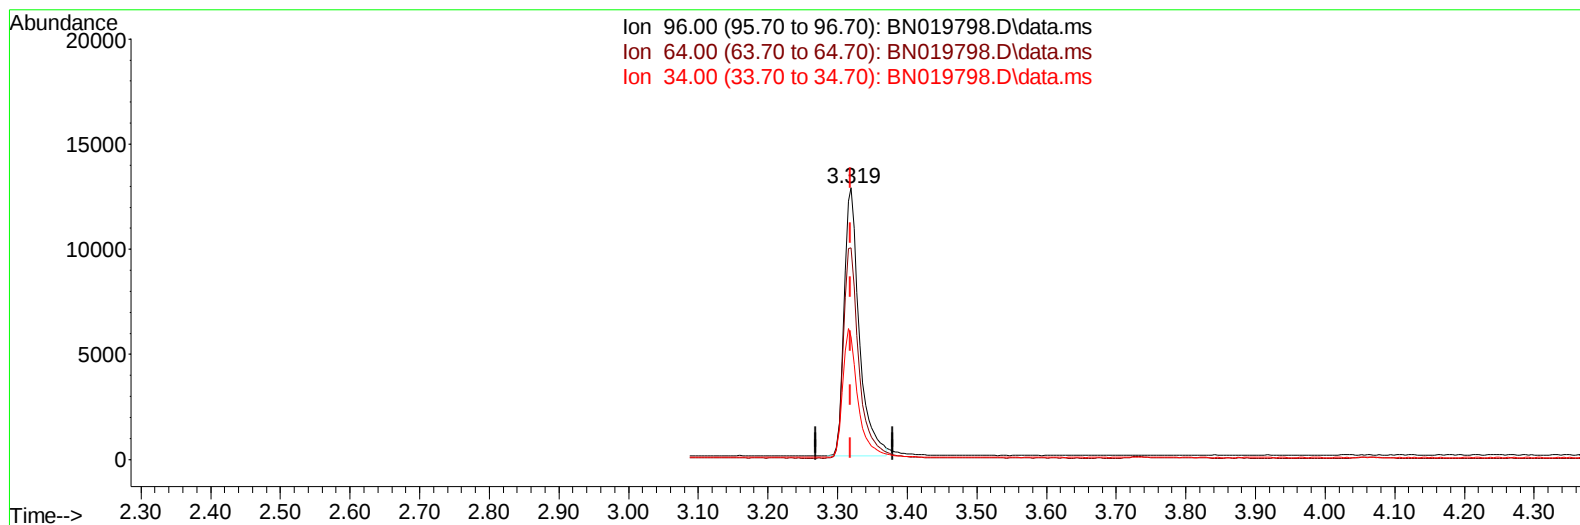

TIC: BN019798.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (+ 0.000) 3.79 ng/ul m

response 19305

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	77.84#
34.00	22.70	45.26#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019798.D
 Acq On : 16 May 2022 18:48
 Operator : CG/JU
 Sample : N2707-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXL99

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 01:43:27 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.855	152		4305	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136		14661	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.479	164		9176	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188		19786	0.400	ng/ul	0.00
17) Chrysene-d12	21.403	240		18604	0.400	ng/ul	0.00
23) Perylene-d12	23.744	264		19264	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.319	96		19305m	3.789	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152		7631	0.344	ng/ul	0.00
18) Fluoranthene-d10	19.244	212		20557	0.349	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
Data File : BN019798.D
Acq On : 16 May 2022 18:48
Operator : CG/JU
Sample : N2707-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXL99

Manual IntegrationsAPPROVED

Quant Time: May 17 01:43:27 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022

