




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
Data File : BN019810.D
Acq On : 17 May 2022 02:39
Operator : CG/JU
Sample : N2831-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB2J9

Manual IntegrationsAPPROVED

Quant Time: May 17 04:11:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022

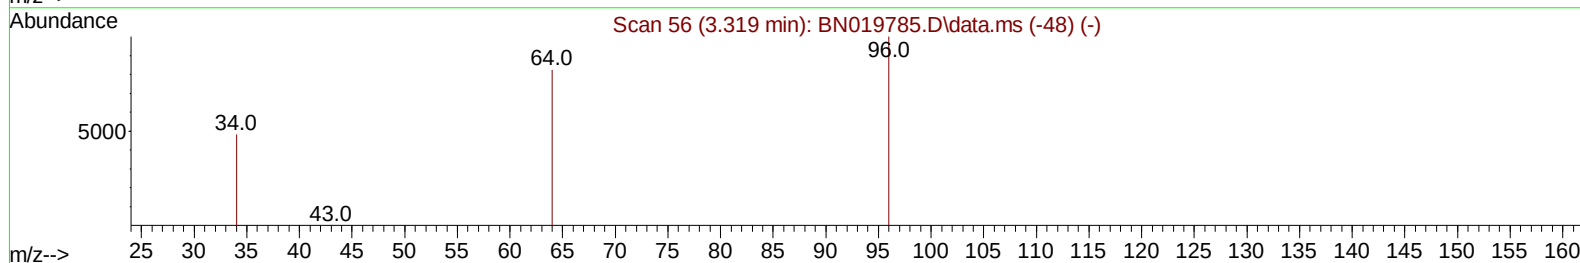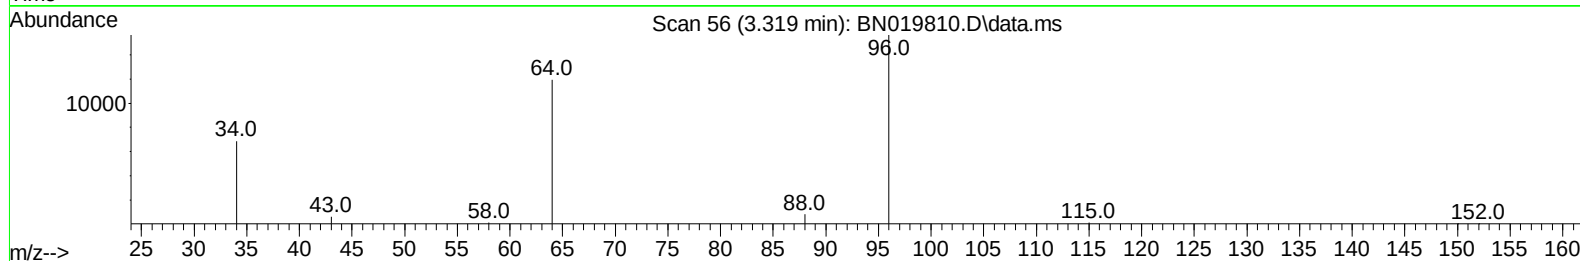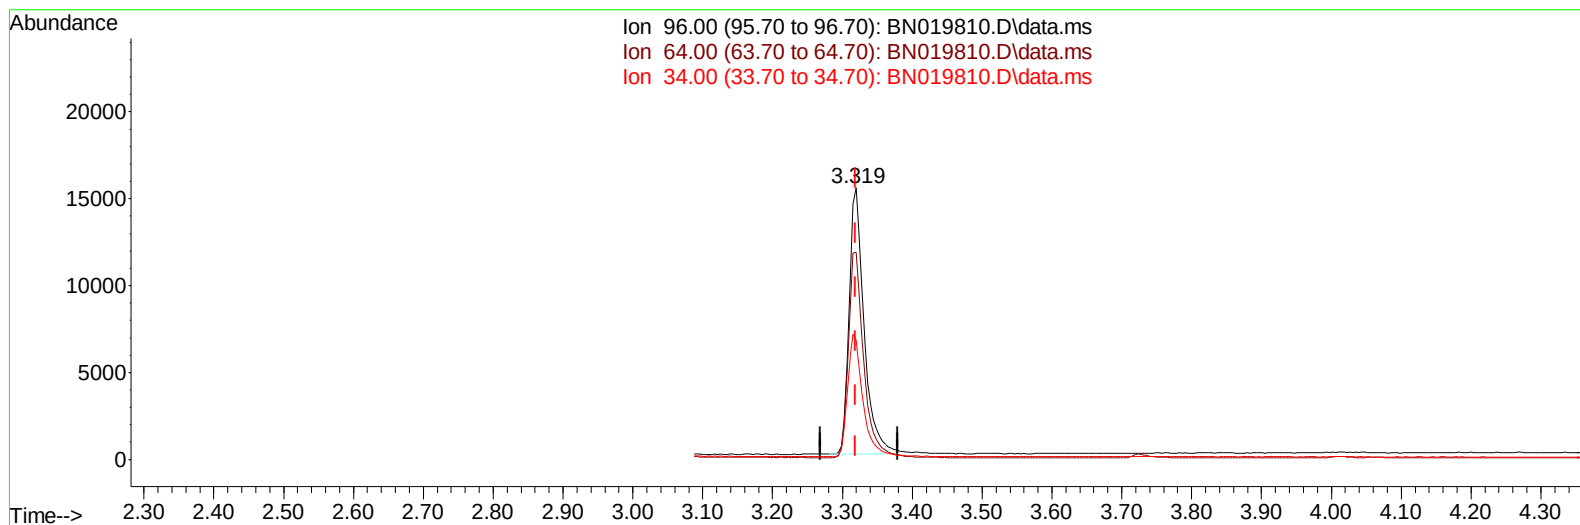

TIC: BN019810.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (+ 0.000) 4.00 ng/u1

response 22478

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.27#
34.00	22.70	44.04#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019810.D
 Acq On : 17 May 2022 02:39
 Operator : CG/JU
 Sample : N2831-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB2J9

Manual IntegrationsAPPROVED

Quant Time: May 17 04:11:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

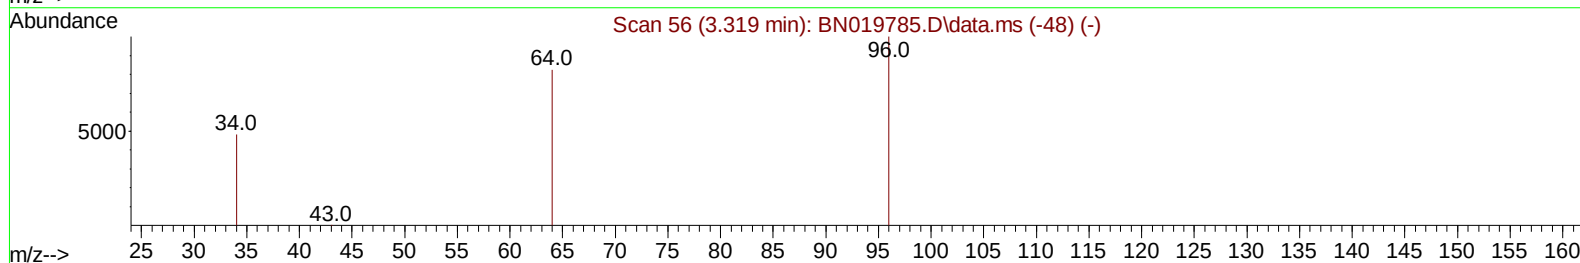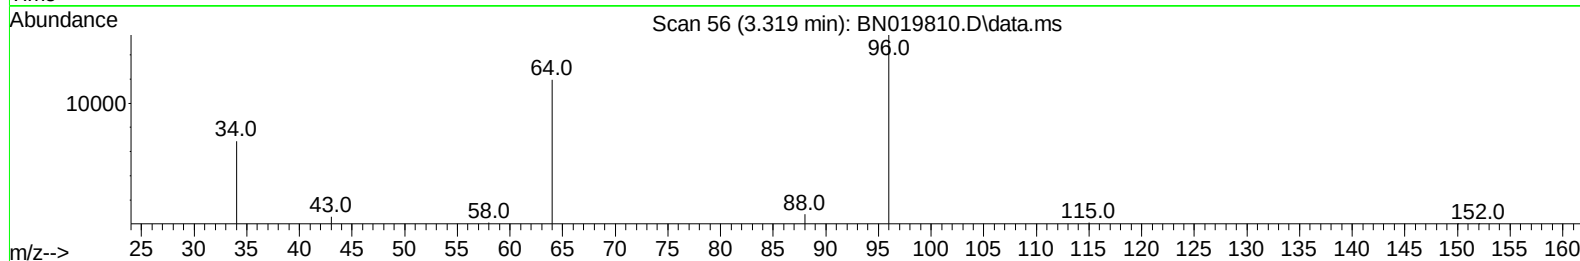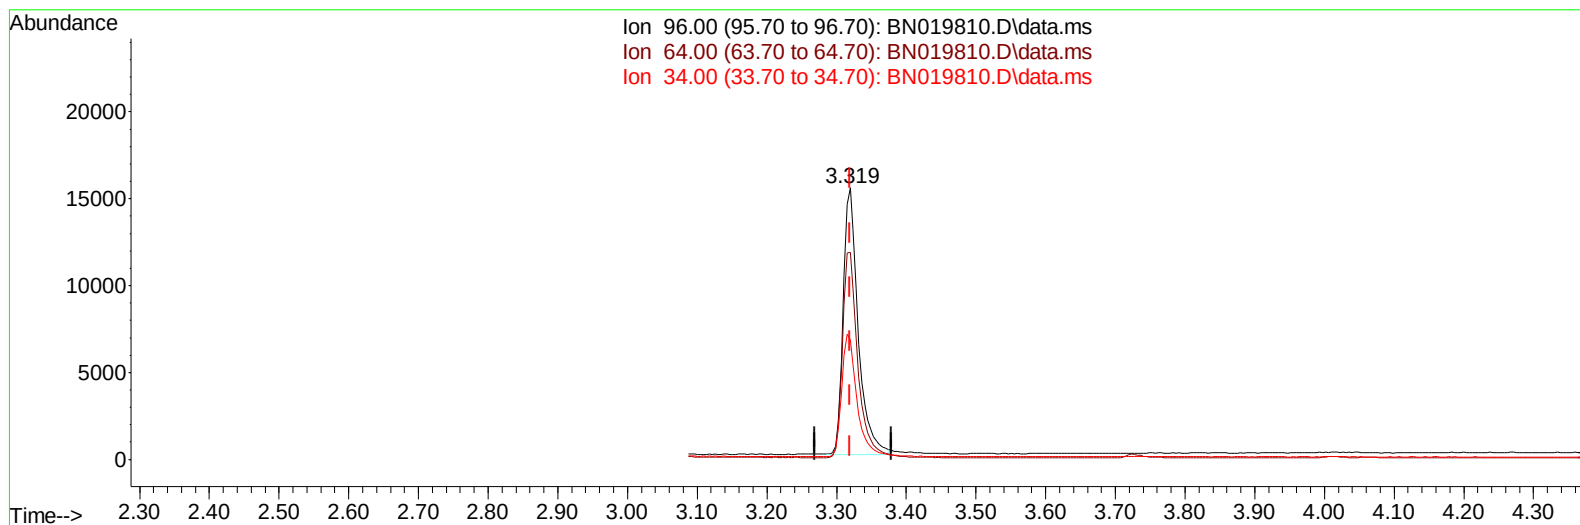

TIC: BN019810.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (+ 0.000) 4.07 ng/ul m

response 22872

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.27#
34.00	22.70	44.04#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019810.D
 Acq On : 17 May 2022 02:39
 Operator : CG/JU
 Sample : N2831-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB2J9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 04:11:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.855	152		4748	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136		16721	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164		11306	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188		24711	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.400	240		22839	0.400	ng/ul	0.00
23) Perylene-d12	23.741	264		20973	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.319	96		22872m	4.070	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152		8371	0.331	ng/ul	0.00
18) Fluoranthene-d10	19.244	212		26322	0.364	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.353	88		463	0.078	ng/ul#	65

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
Data File : BN019810.D
Acq On : 17 May 2022 02:39
Operator : CG/JU
Sample : N2831-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB2J9

Manual IntegrationsAPPROVED

Quant Time: May 17 04:11:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022

