

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019804.D
 Acq On : 16 May 2022 23:03
 Operator : CG/JU
 Sample : N2831-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB2K2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 01:43:46 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	4650	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136	16135	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164	10611	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	23160	0.400	ng/ul	0.00
17) Chrysene-d12	21.400	240	22436	0.400	ng/ul	0.00
23) Perylene-d12	23.738	264	21082	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	24740m	4.496	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	6763	0.277	ng/ul	0.00
18) Fluoranthene-d10	19.244	212	19602	0.276	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.353	88	6888m	1.179	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
Data File : BN019804.D
Acq On : 16 May 2022 23:03
Operator : CG/JU
Sample : N2831-05
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
YB2K2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022


Quant Time: May 17 01:43:46 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

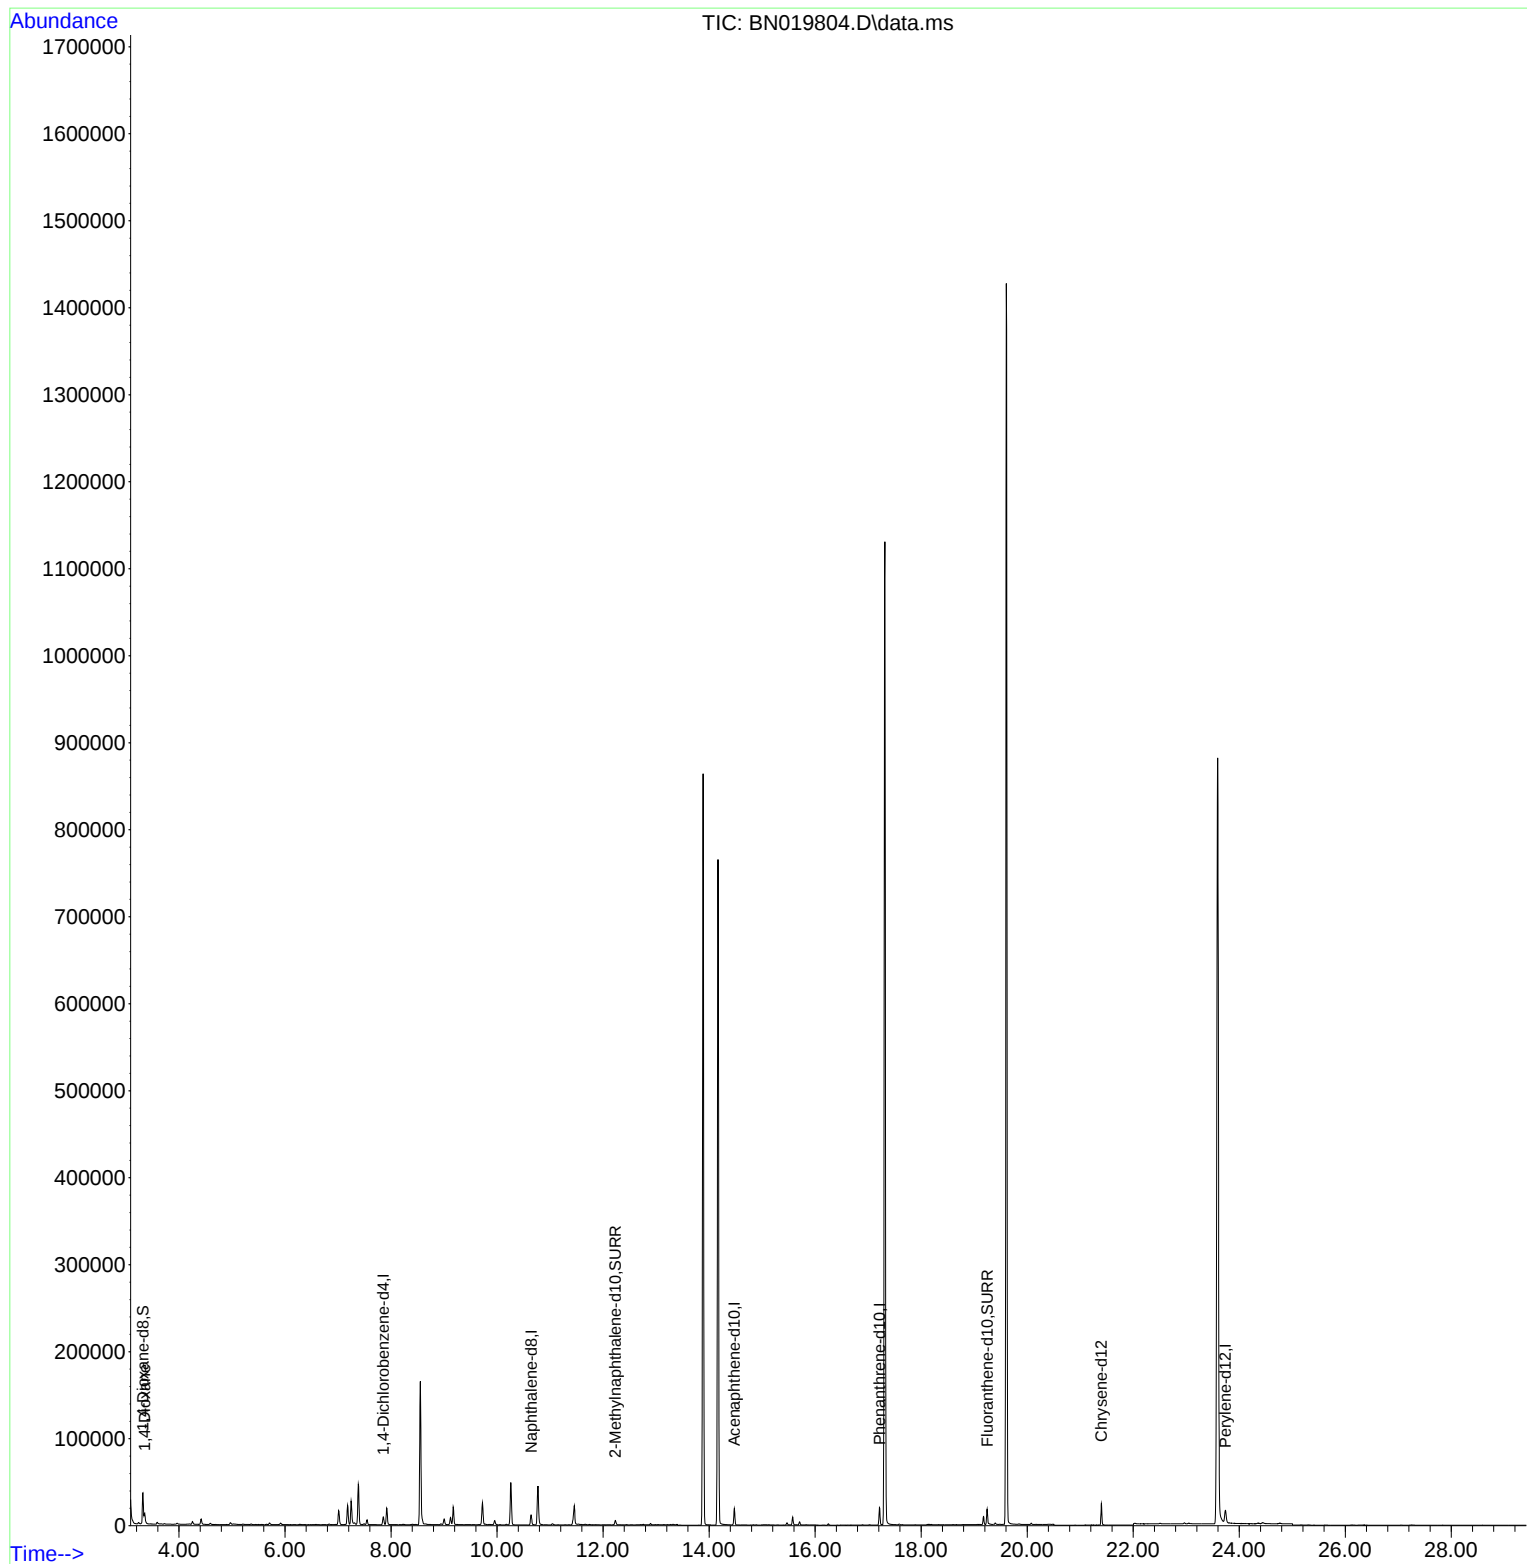

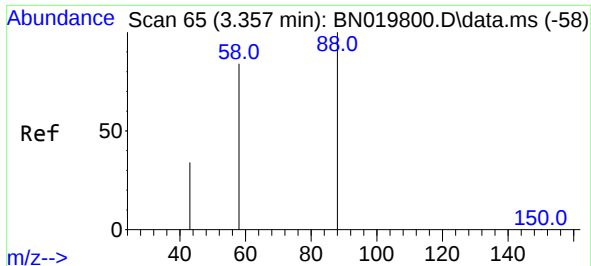

#2
 1,4-Dioxane
 Concen: 1.179 ng/ul m
 RT: 3.353 min Scan# 64
 Delta R.T. -0.004 min
 Lab File: BN019804.D
 Acq: 16 May 2022 23:03

Instrument :
 BNA_N
 ClientSampleId :
 YB2K2

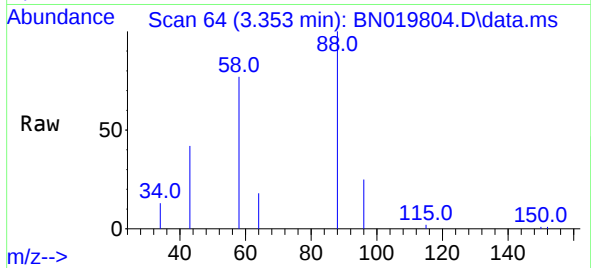

Tgt Ion: 88 Resp: 688
 Ion Ratio Lower Upper
 88 100
 43 41.6 39.0 58.4
 58 77.2 39.8 59.8

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

