

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019805.D
 Acq On : 16 May 2022 23:39
 Operator : CG/JU
 Sample : N2831-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB2K3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 01:43:49 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	4593	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136	16212	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164	10838	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	23618	0.400	ng/ul	0.00
17) Chrysene-d12	21.398	240	22377	0.400	ng/ul	0.00
23) Perylene-d12	23.737	264	20641	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	24488m	4.505	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	9270	0.378	ng/ul	0.00
18) Fluoranthene-d10	19.253	212	22860	0.323	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.353	88	3349	0.580	ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
Data File : BN019805.D
Acq On : 16 May 2022 23:39
Operator : CG/JU
Sample : N2831-06
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
YB2K3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022


Quant Time: May 17 01:43:49 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

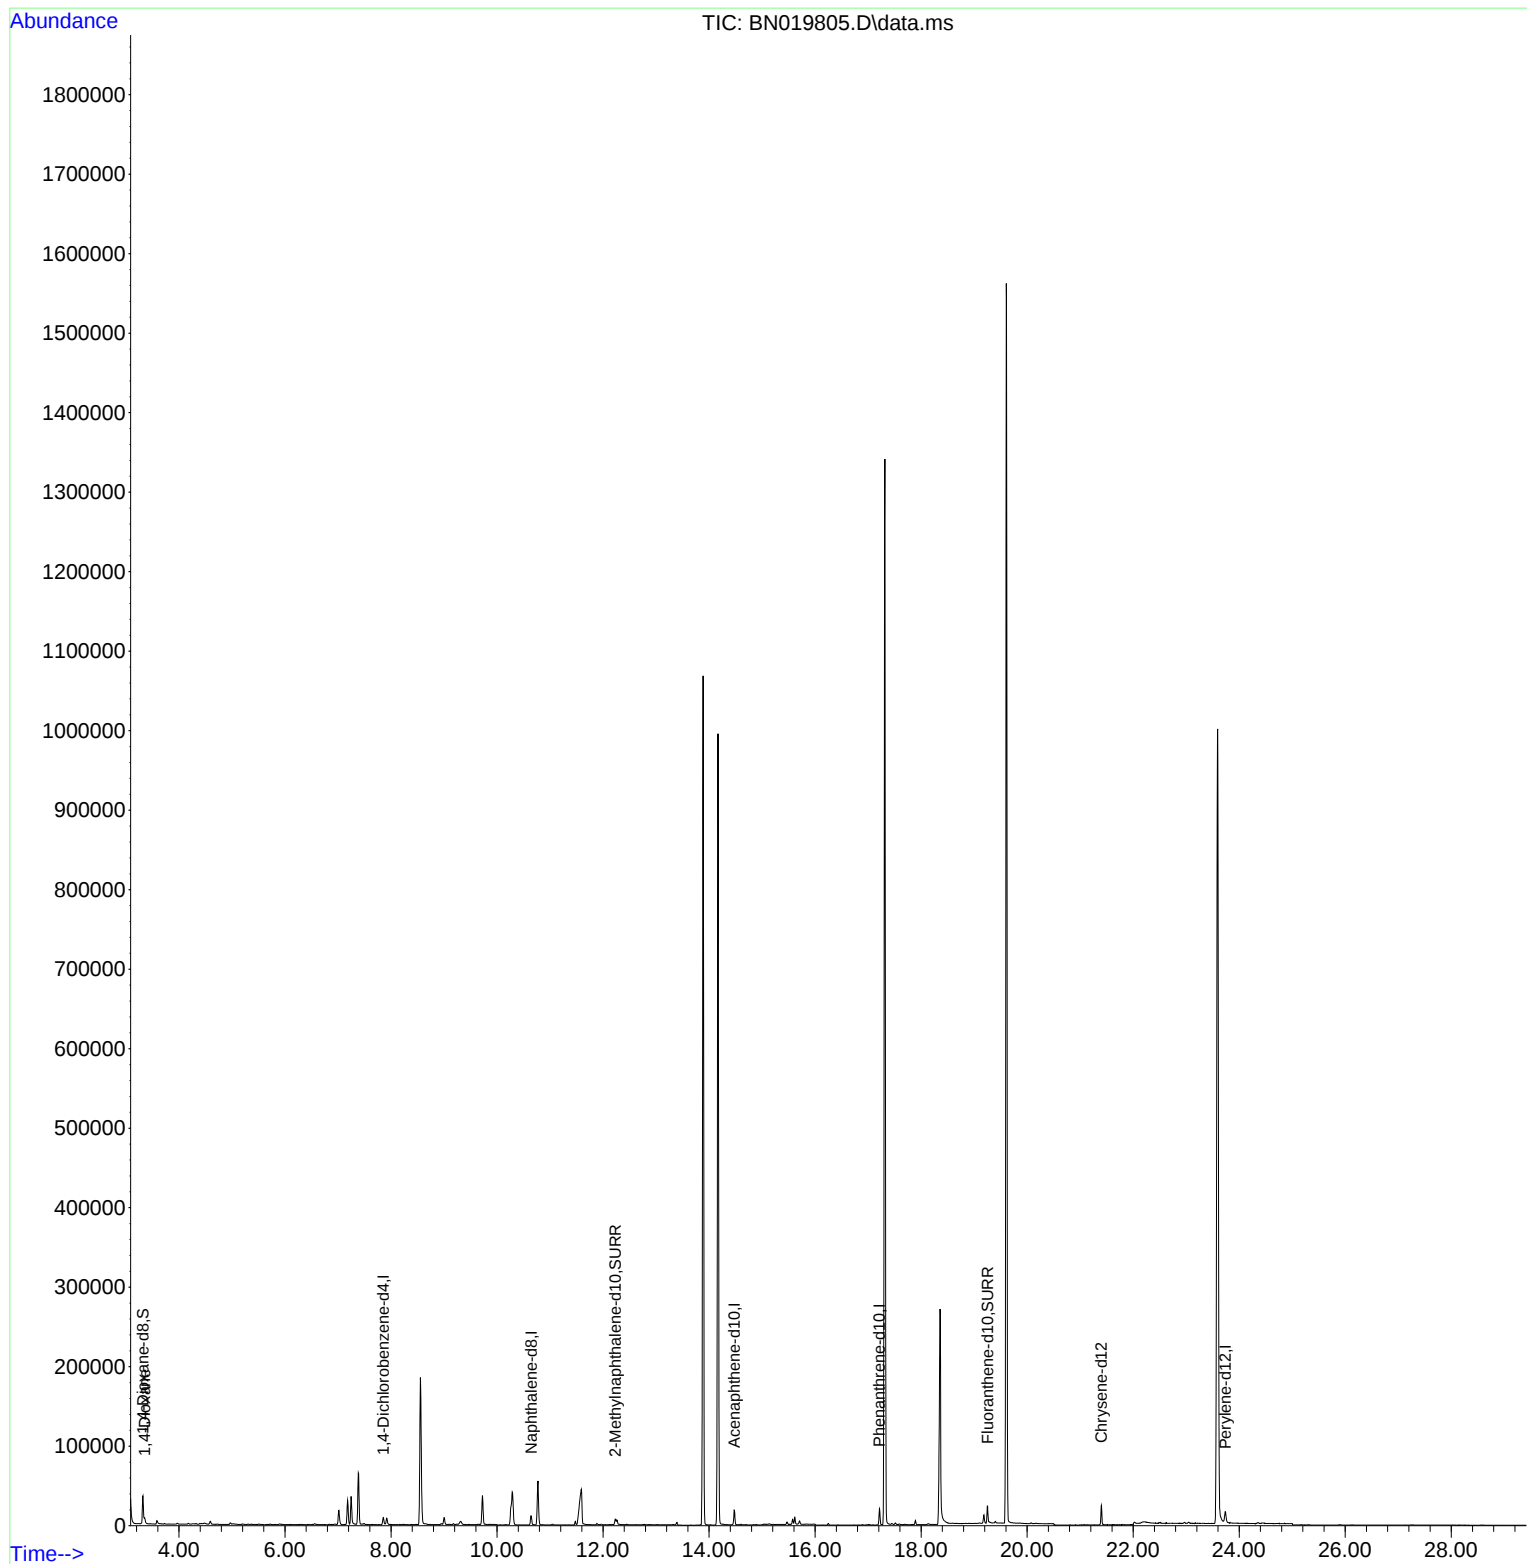

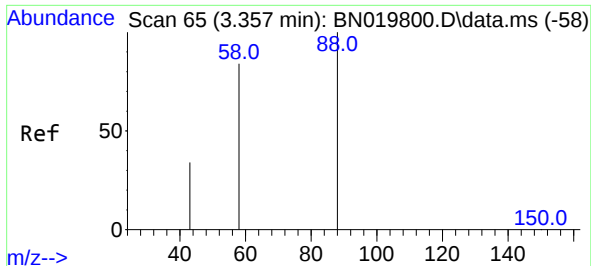

#2
 1,4-Dioxane
 Concen: 0.580 ng/ul
 RT: 3.353 min Scan# 64
 Delta R.T. -0.004 min
 Lab File: BN019805.D
 Acq: 16 May 2022 23:39

Instrument :
 BNA_N
 ClientSampleId :
 YB2K3

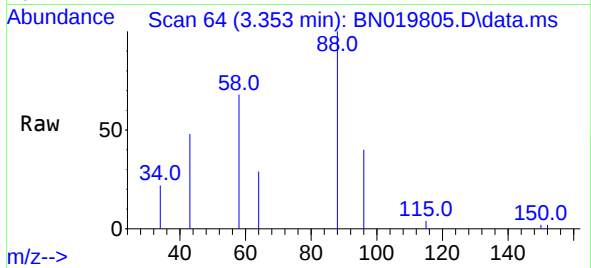

Tgt Ion: 88 Resp: 3349
 Ion Ratio Lower Upper
 88 100
 43 47.6 39.0 58.4
 58 67.7 39.8 59.8

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

