

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
 Data File : BN019808.D
 Acq On : 17 May 2022 01:27
 Operator : CG/JU
 Sample : N2831-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB2K0

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 04:10:55 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	4243	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	14690	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164	9761	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	21859	0.400	ng/ul	0.00
17) Chrysene-d12	21.397	240	21373	0.400	ng/ul	0.00
23) Perylene-d12	23.735	264	20327	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	22537m	4.488	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	8375	0.377	ng/ul	0.00
18) Fluoranthene-d10	19.244	212	26723	0.395	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.353	88	7281m	1.366	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051622\
Data File : BN019808.D
Acq On : 17 May 2022 01:27
Operator : CG/JU
Sample : N2831-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB2K0




Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 04:10:55 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

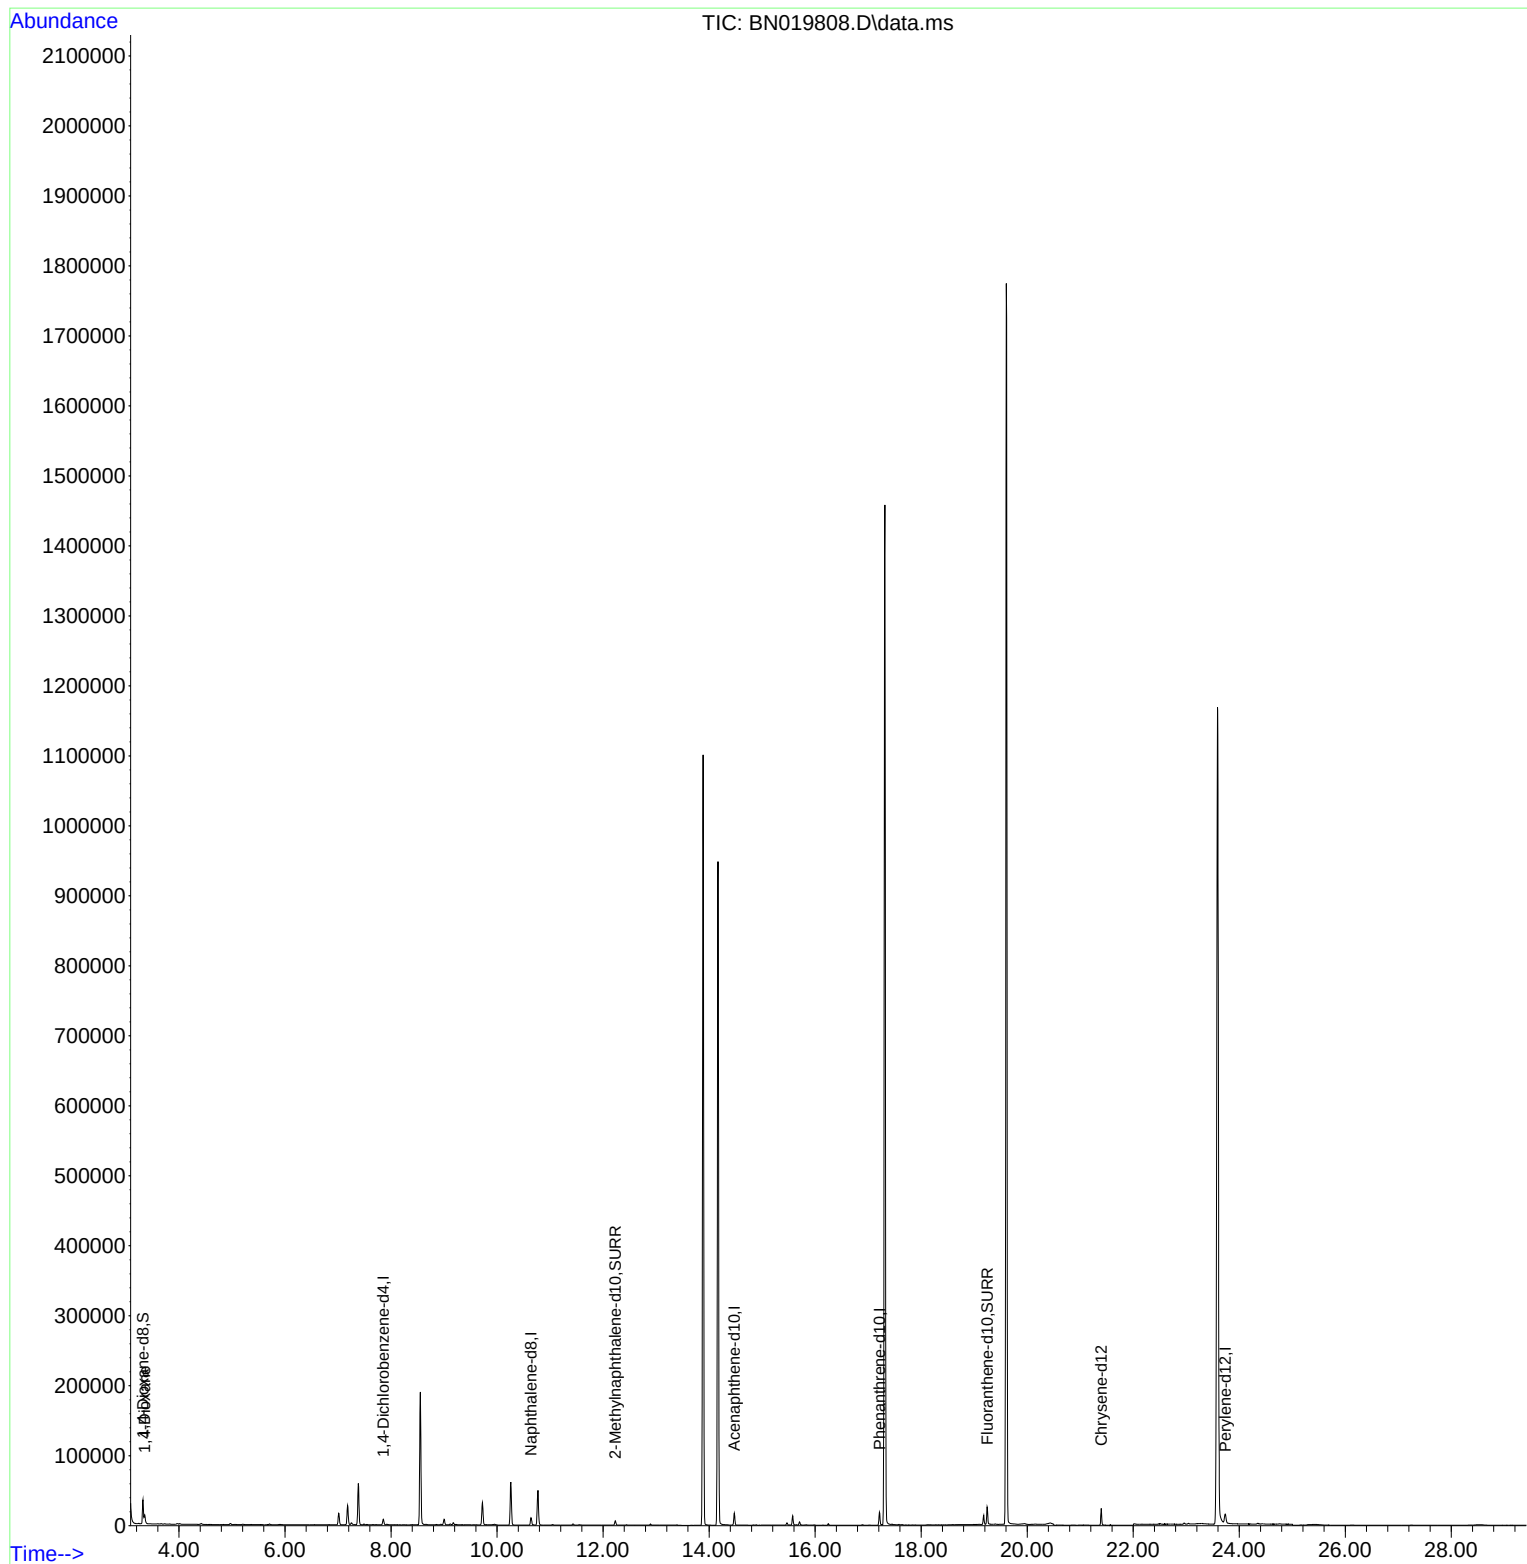

Abundance Scan 65 (3.357 min): BN019800.D\data.ms (-58)

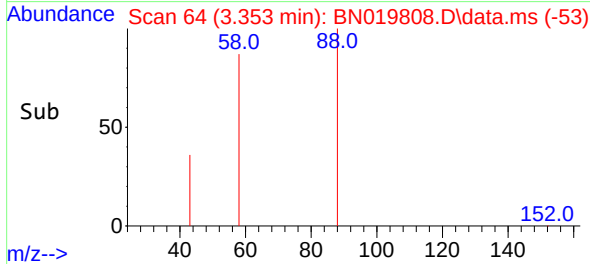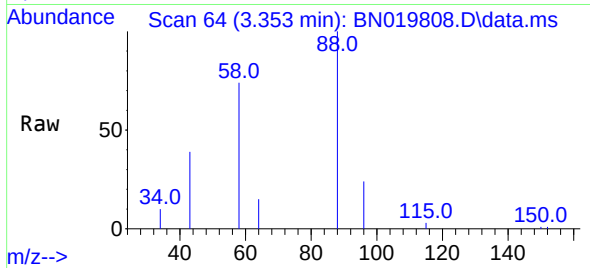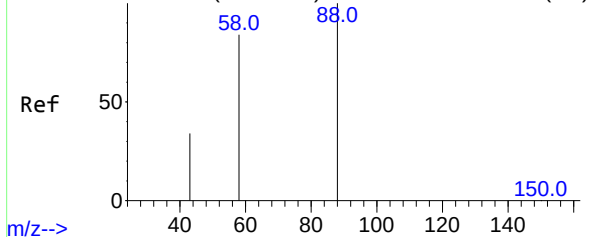

#2
1,4-Dioxane
Concen: 1.366 ng/ul m
RT: 3.353 min Scan# 64
Delta R.T. -0.004 min
Lab File: BN019808.D
Acq: 17 May 2022 01:27

Tgt Ion: 88 Resp: 728
Ion Ratio Lower Upper
88 100
43 39.2 39.0 58.4
58 74.1 39.8 59.8

Instrument :
BNA_N
ClientSampleId :
YB2K0

Manual Integrations
APPROVED
Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022

