
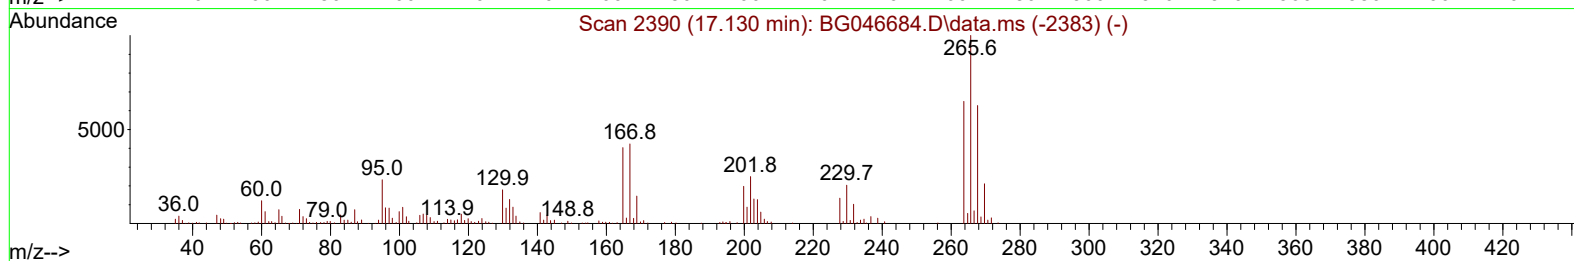
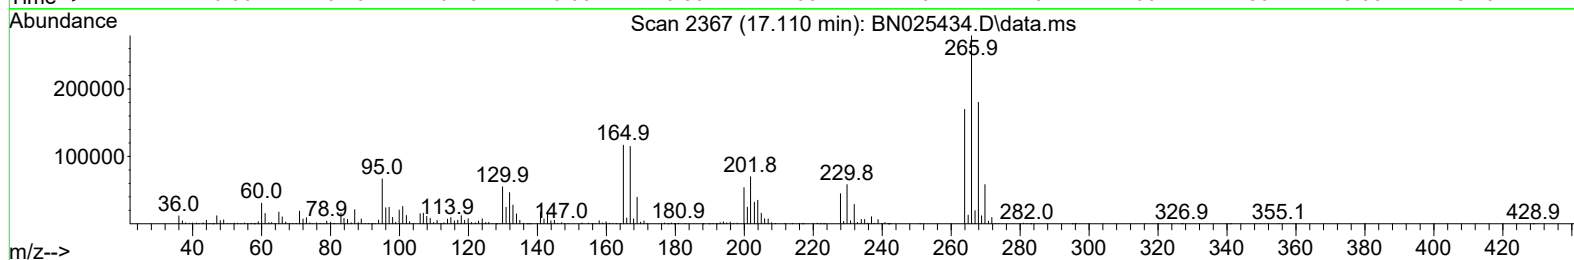


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051623\
Data File : BN025434.D
Acq On : 16 May 2023 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 05:24:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 17 05:24:30 2023
Response via : Initial Calibration

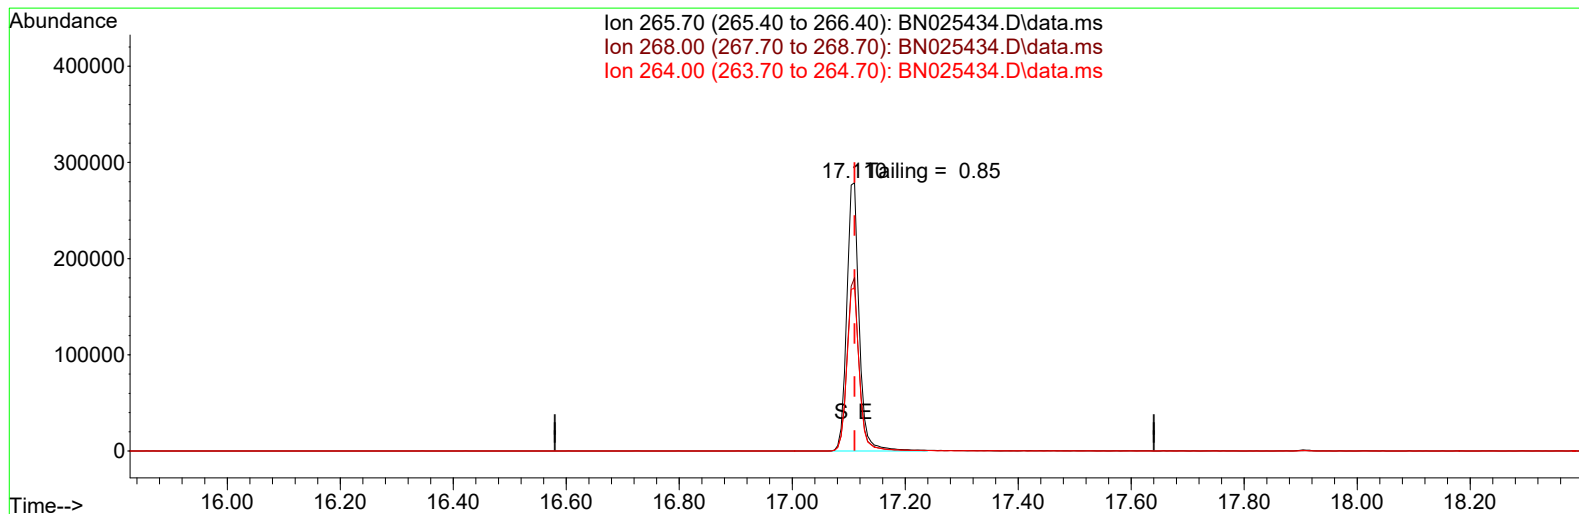

TIC: BN025434.D\data.ms

(70) Pentachlorophenol (C)




17.110min (0.000) 19391.19 ng

response 426857

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.58
264.00	61.60	60.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051623\
Data File : BN025434.D
Acq On : 16 May 2023 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 05:24:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 17 05:24:30 2023
Response via : Initial Calibration

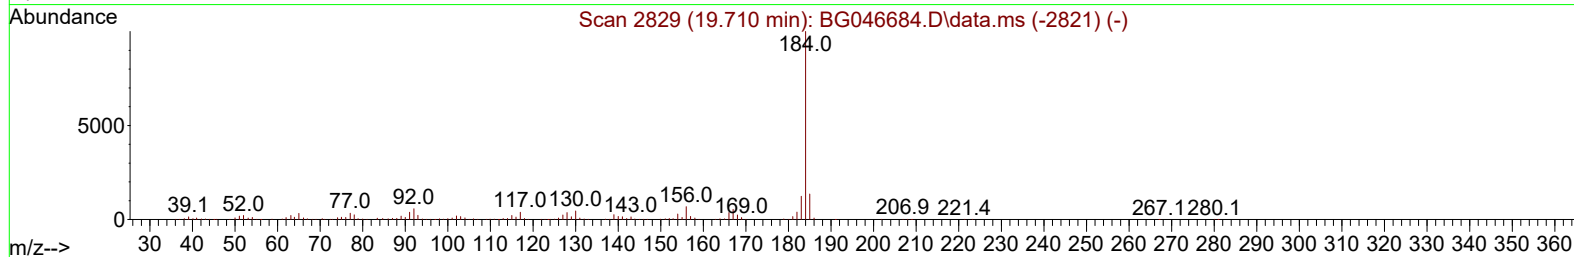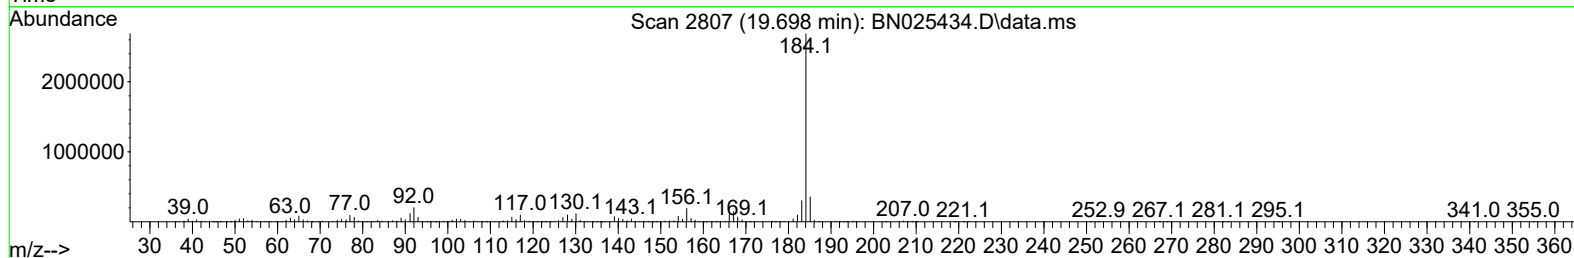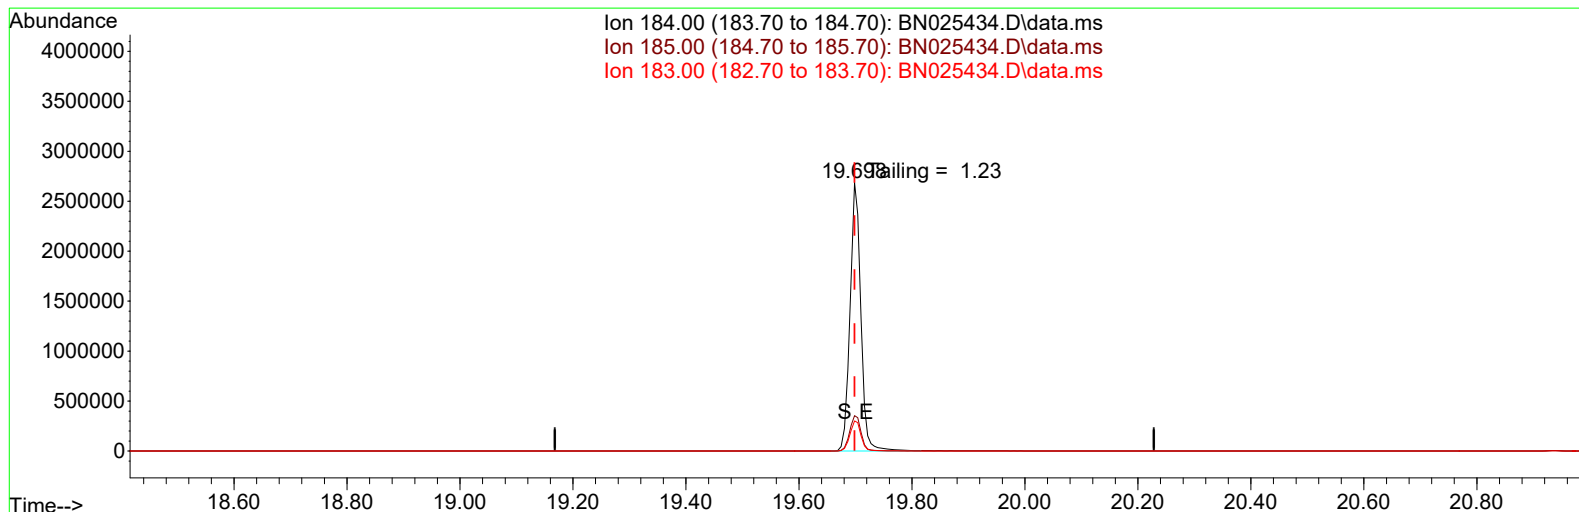

TIC: BN025434.D\data.ms

(77) Benzidine**19.698min (0.000) 2067068.11 ng****response 3568216**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.19
183.00	13.20	11.25
0.00	0.00	0.00