
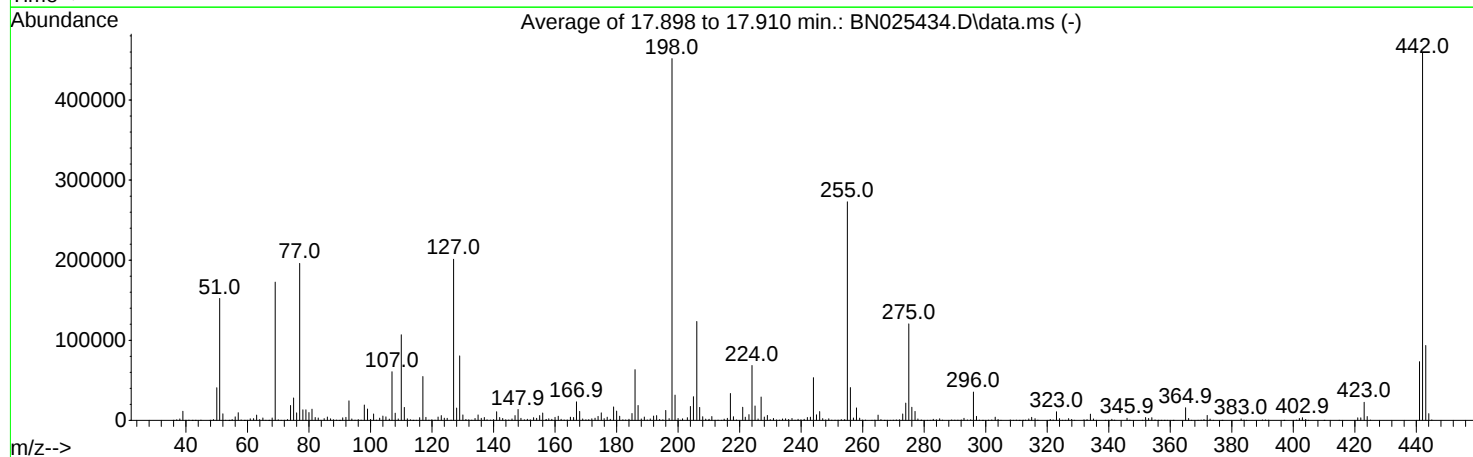


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051623\
 Data File : BN025434.D
 Acq On : 16 May 2023 09:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 17 02:52:36 2023

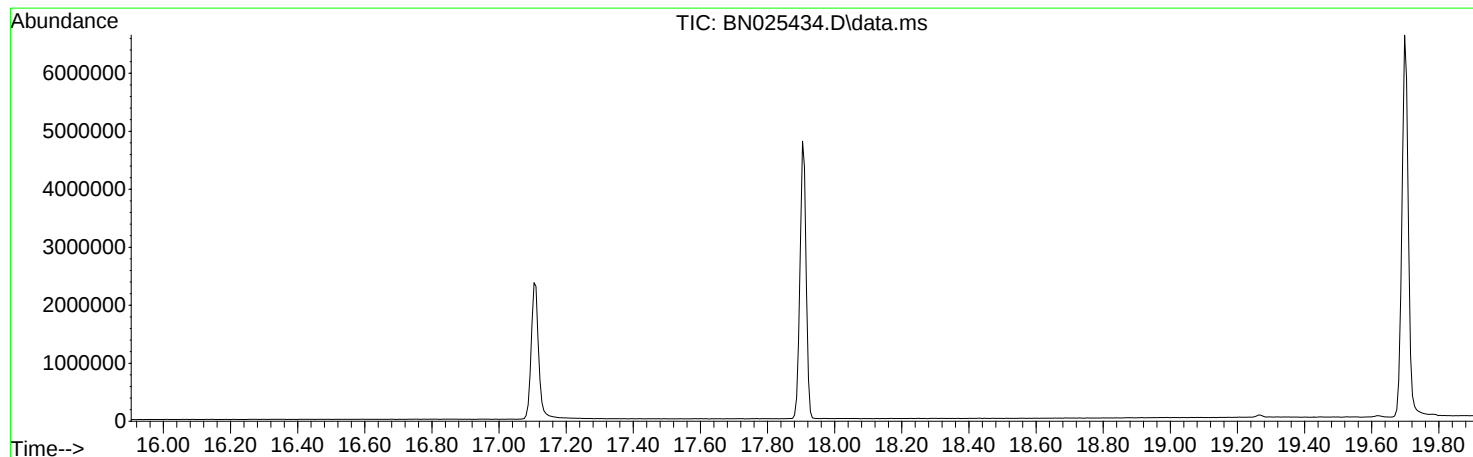

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	152172	PASS
68	69	0.00	2	1.8	3082	PASS
69	198	0.00	100	38.2	172676	PASS
70	69	0.00	2	0.5	862	PASS
127	198	10	80	44.6	201259	PASS
197	198	0.00	2	0.5	2187	PASS
198	198	100	100	100.0	451648	PASS
199	198	5	9	7.0	31491	PASS
275	198	10	60	26.7	120504	PASS
365	198	1	100	3.5	15787	PASS
441	198	0.01	100	16.2	73325	PASS
442	442	50	100	100.0	459328	PASS
443	442	15	24	20.4	93485	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/16/2023	BNA_N	<u>BN025434.D</u>
Compound Name	Response	Retention Time
DDT	1538777	20.939
DDD	15120	20.551
DDE	67	20.104
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15187	1553964	0.98

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051623\
Data File : BN025434.D
Acq On : 16 May 2023 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 17 05:24:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 17 05:24:30 2023
Response via : Initial Calibration

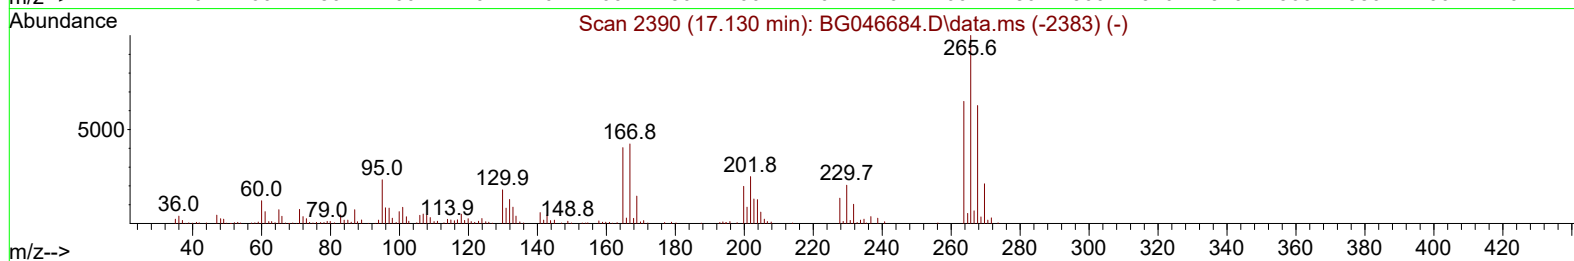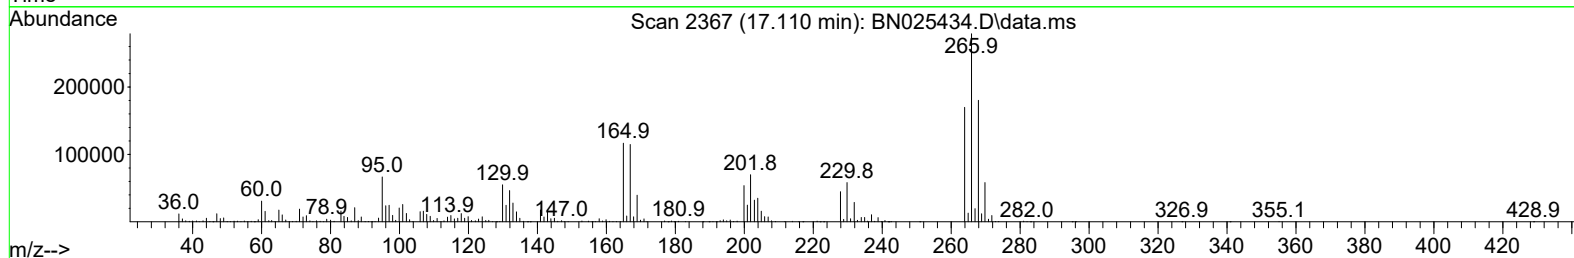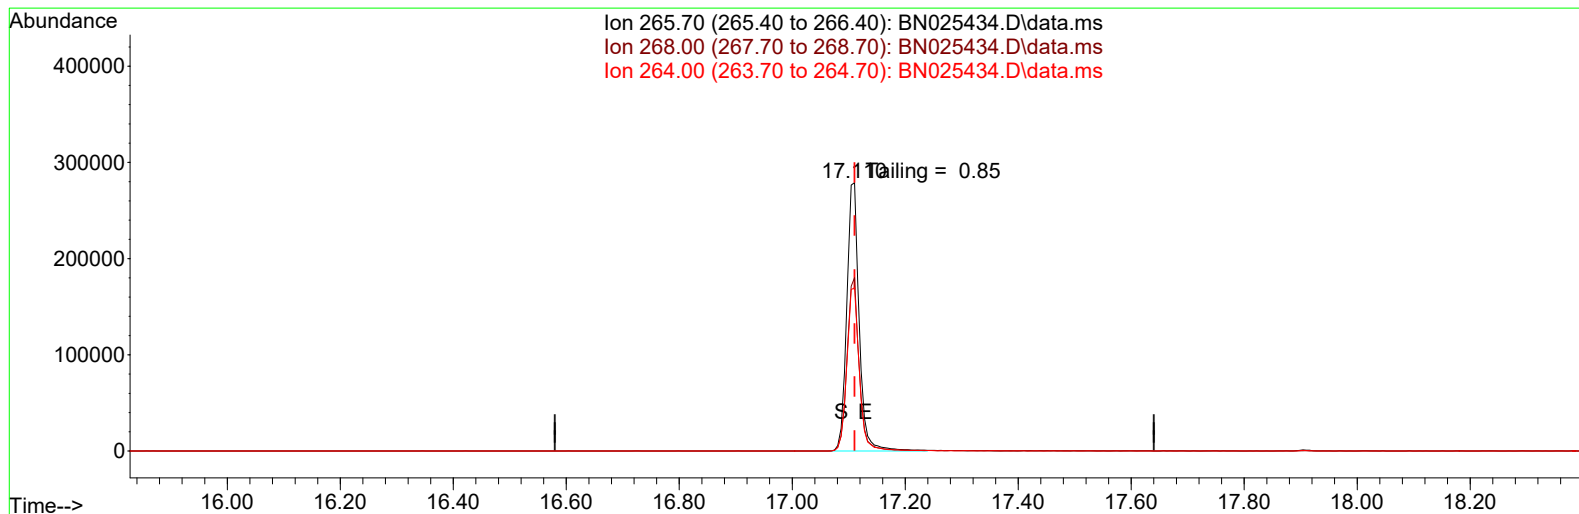

TIC: BN025434.D\data.ms

(70) Pentachlorophenol (C)

17.110min (0.000) 19391.19 ng




response 426857

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.58
264.00	61.60	60.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051623\
Data File : BN025434.D
Acq On : 16 May 2023 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 17 05:24:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 17 05:24:30 2023
Response via : Initial Calibration

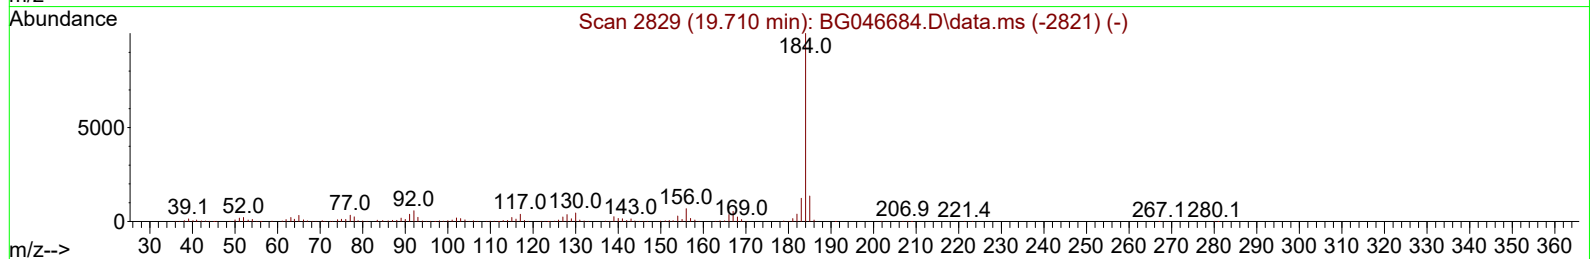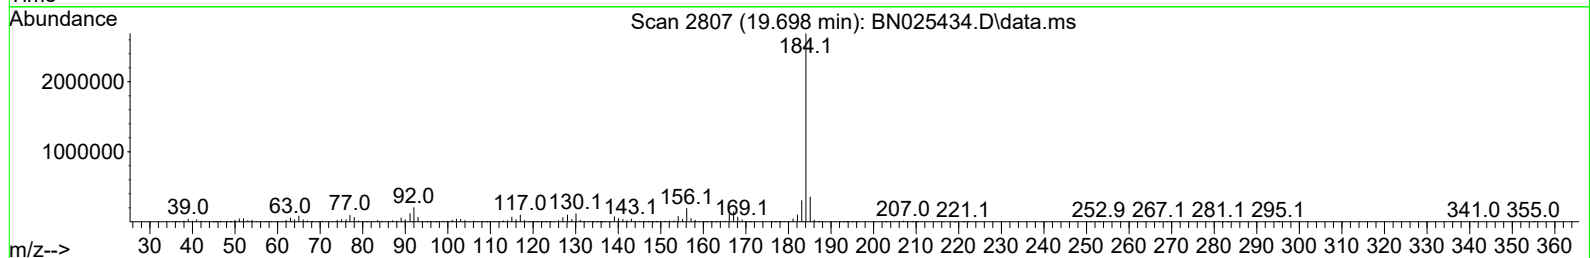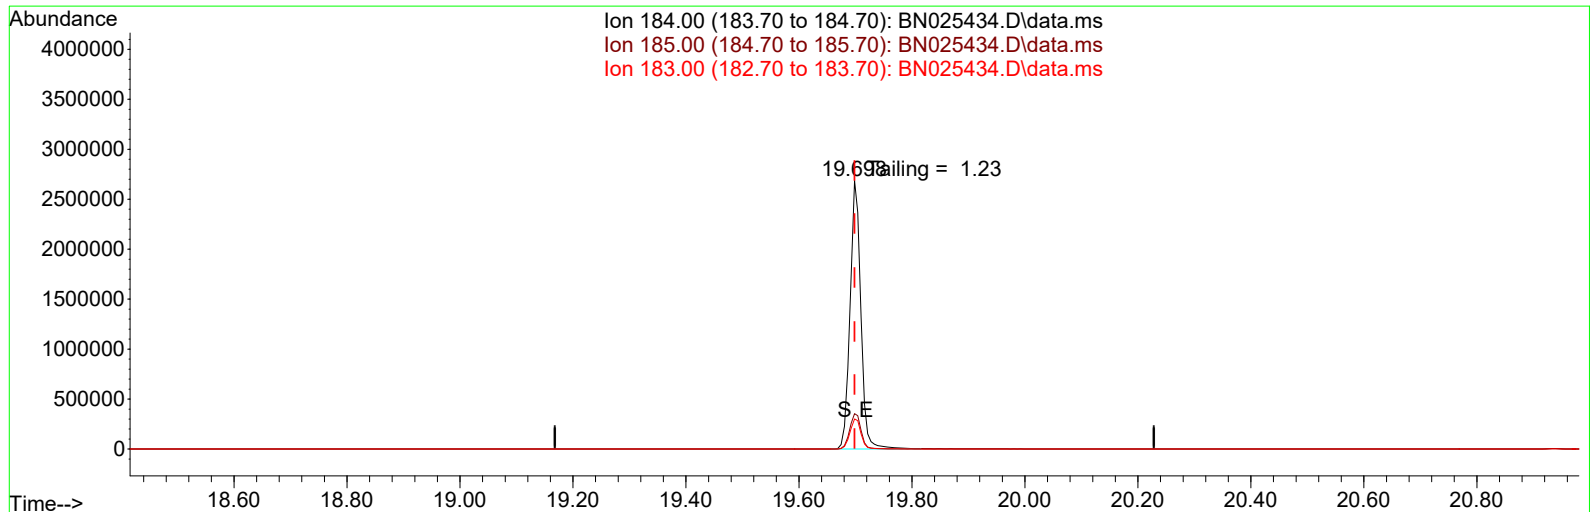

TIC: BN025434.D\data.ms

(77) Benzidine

19.698min (0.000) 2067068.11 ng

response 3568216

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.19
183.00	13.20	11.25
0.00	0.00	0.00