

Quantitation Report (QT Reviewed)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051721\
 Data File : BN014658.D
 Acq On : 17 May 2021 18:32
 Operator : CG/JU
 Sample : M2427-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG1Z5

Quant Time: May 18 12:21:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 15:50:11 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 5/19/2021 11:38:17 AM

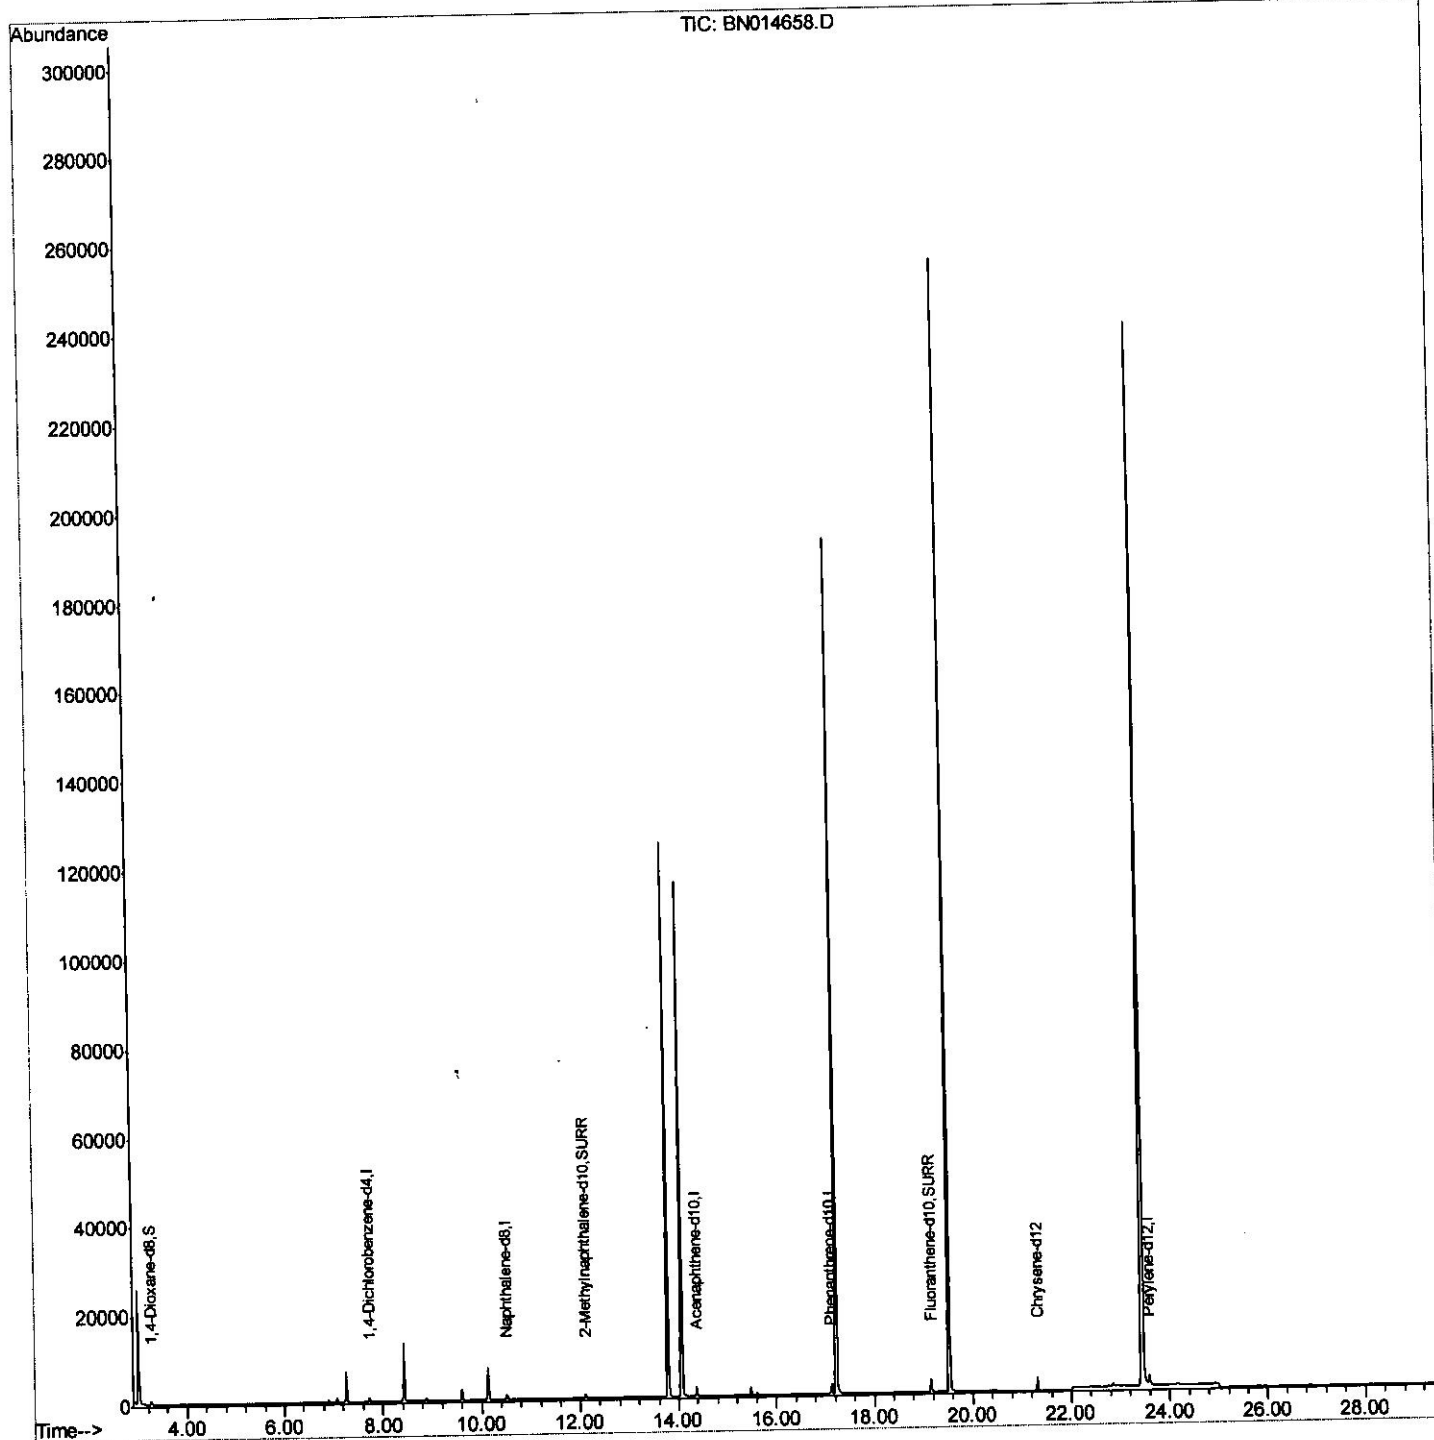

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051721\
 Data File : BN014658.D
 Acq On : 17 May 2021 18:32
 Operator : CG/JU
 Sample : M2427-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG1Z5

Manual Integrations
 APPROVED

mohammad
 5/19/2021 11:38:17 AM

Quant Time: May 18 12:17:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 15:50:11 2021
 Response via : Initial Calibration

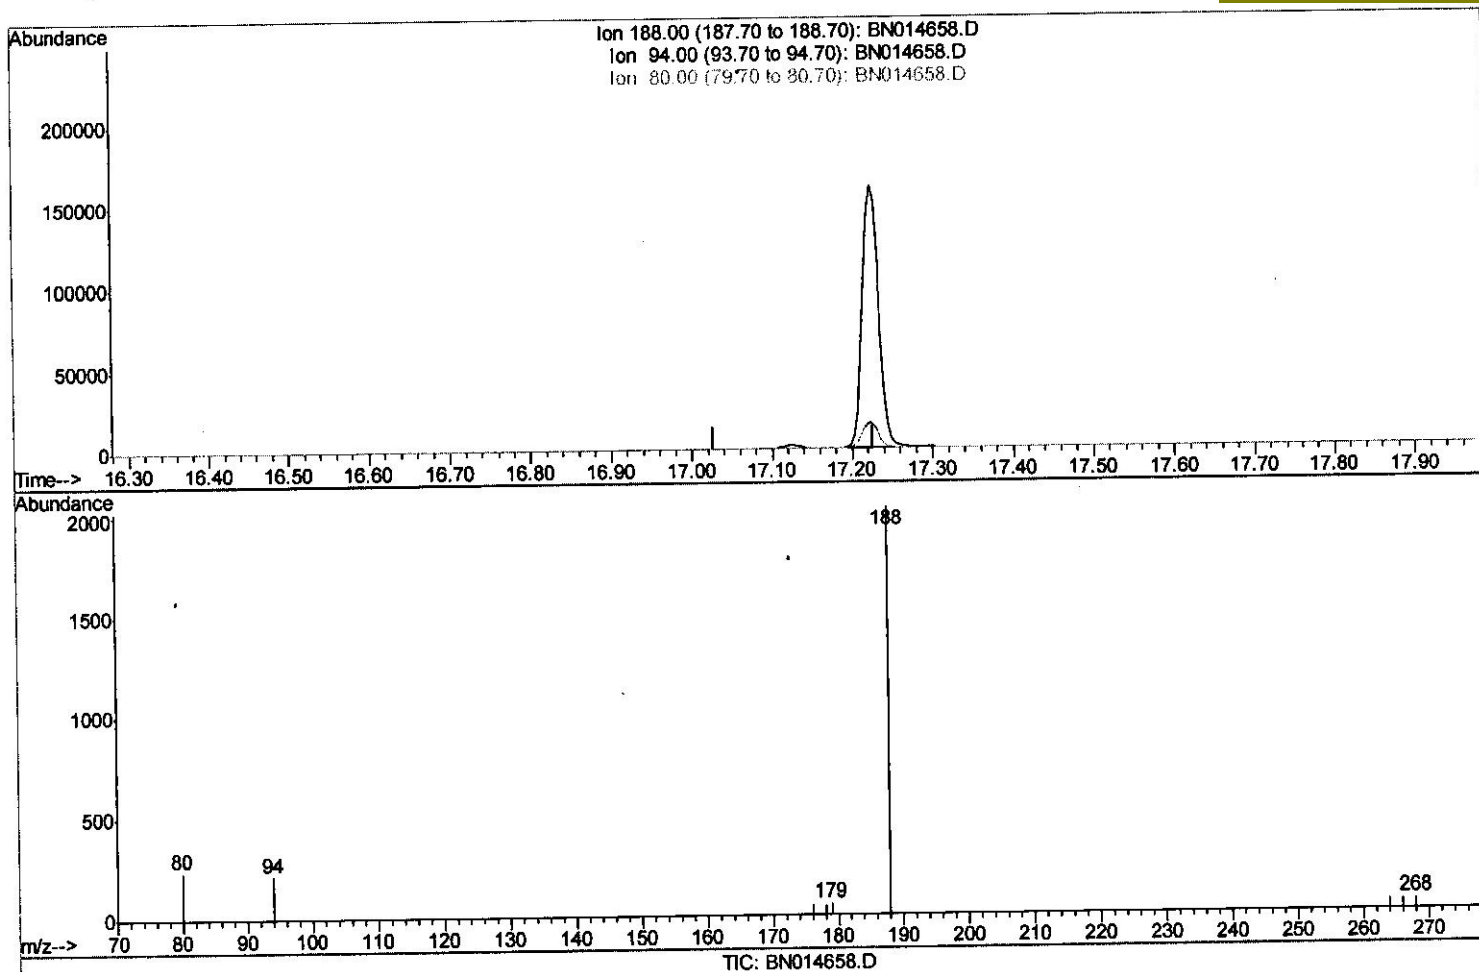

(13) Phenanthrene-d10 (I)

17.127min (-17.127) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.10	0.00#
80.00	12.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051721\
 Data File : BN014658.D
 Acq On : 17 May 2021 18:32
 Operator : CG/JU
 Sample : M2427-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG1Z5

Manual Integrations
 APPROVED

mohammad
 5/19/2021 11:38:17 AM

Quant Time: Mav 18 12:17:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 15:50:11 2021
 Response via : Initial Calibration

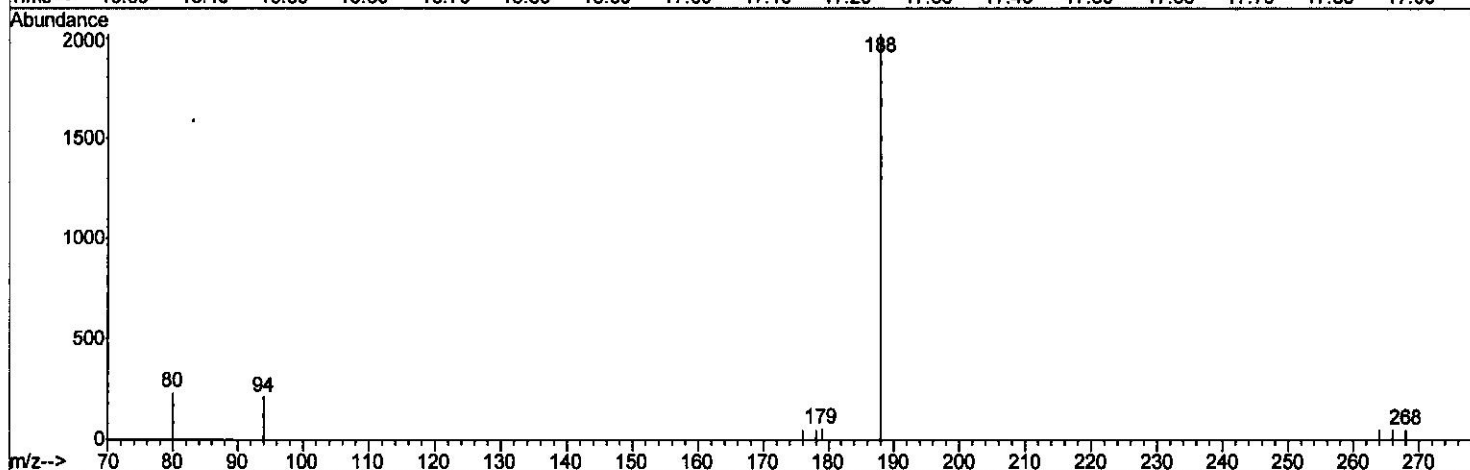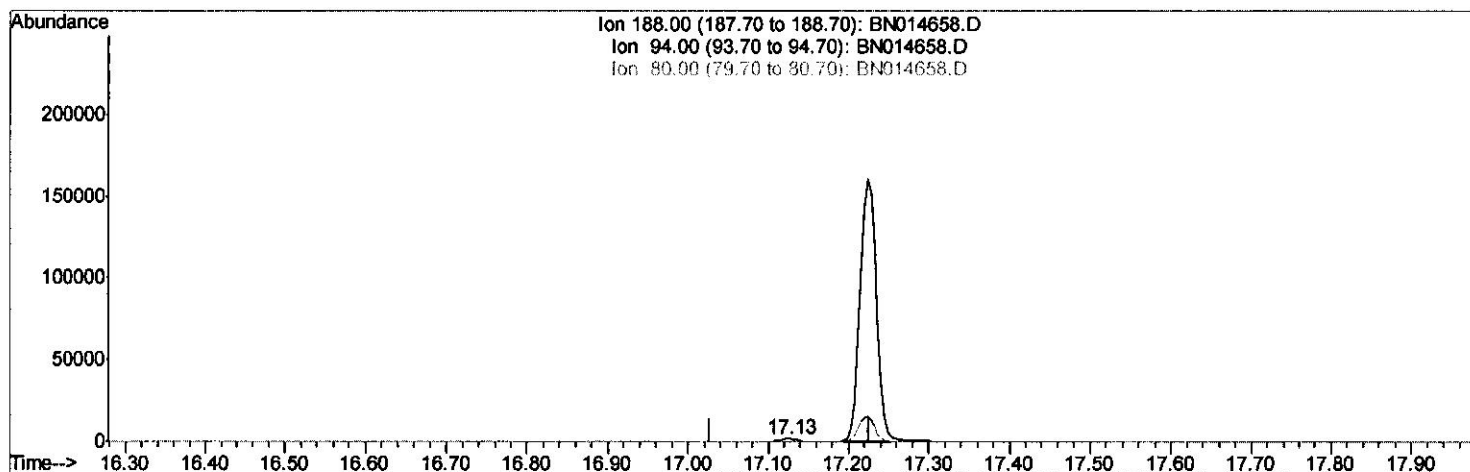

(13) Phenanthrene-d10 (I)

17.127min (-0.000) 0.40ng/ul m

response 2899

Ion	Exp%	Act%
188.00	100	100
94.00	11.10	10.53
80.00	12.50	11.57
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051721\
Data File : BN014658.D
Acq On : 17 May 2021 18:32
Operator : CG/JU
Sample : M2427-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG1Z5

Manual Integrations
APPROVED

mohammad
5/19/2021 11:38:17 AM

Quant Time: May 18 12:21:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 15:50:11 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	466	0.40	ng/ul	0.00
4) Naphthalene-d8	10.52	136	1531	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.38	164	1206	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.13	188	2899m	0.40	ng/ul	0.00
17) Chrysene-d12	21.32	240	3014	0.40	ng/ul	0.00
23) Perylene-d12	23.59	264	3209	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	557	1.17	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.11	152	937	0.35	ng/ul	0.00
18) Fluoranthene-d10	19.16	212	3483	0.46	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

5/19/21 JV