
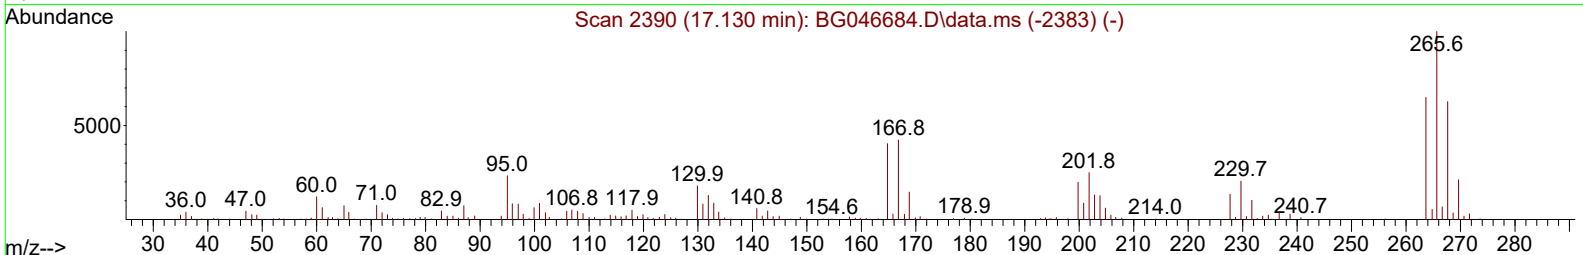
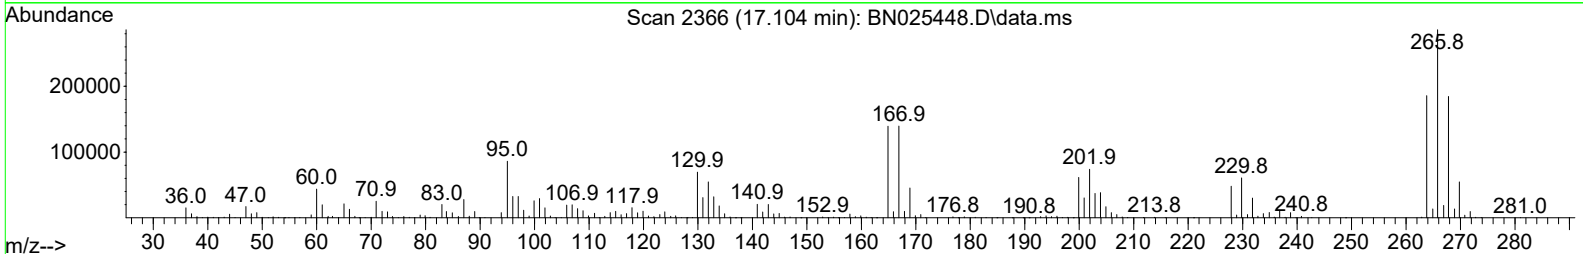


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN051723\  
 Data File : BN025448.D  
 Acq On : 17 May 2023 09:27  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 05:36:54 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu May 18 05:36:50 2023  
 Response via : Initial Calibration

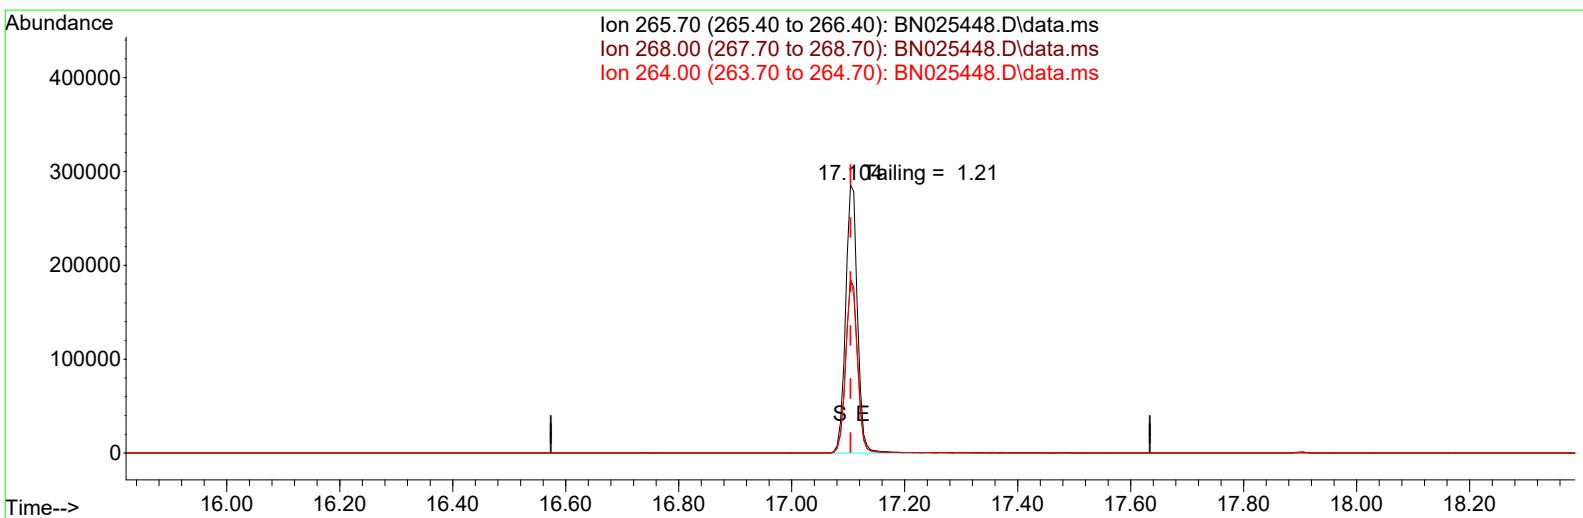

TIC: BN025448.D\data.ms




(70) Pentachlorophenol (C)

17.104min ( 0.000) 17533.93 ng

response	418585
Ion	Exp% Act%
265.70	100.00 100.00
268.00	62.20 64.50
264.00	61.60 64.95
0.00	0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN051723\  
 Data File : BN025448.D  
 Acq On : 17 May 2023 09:27  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 05:36:54 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu May 18 05:36:50 2023  
 Response via : Initial Calibration

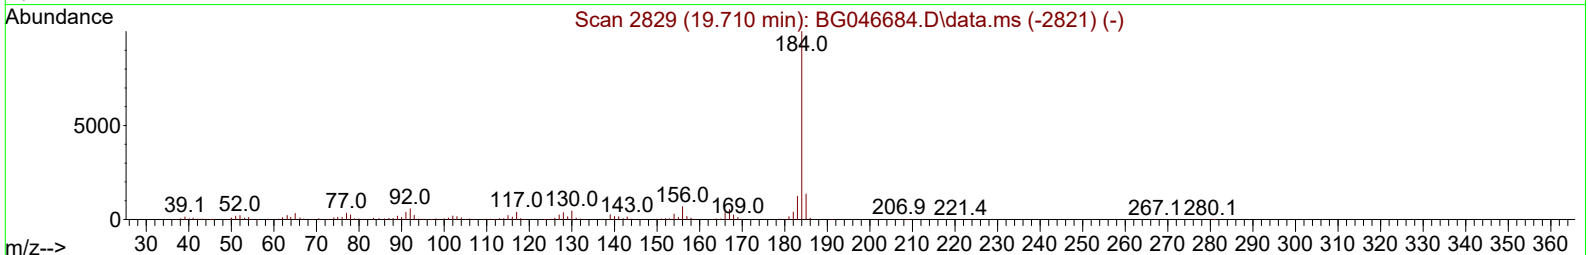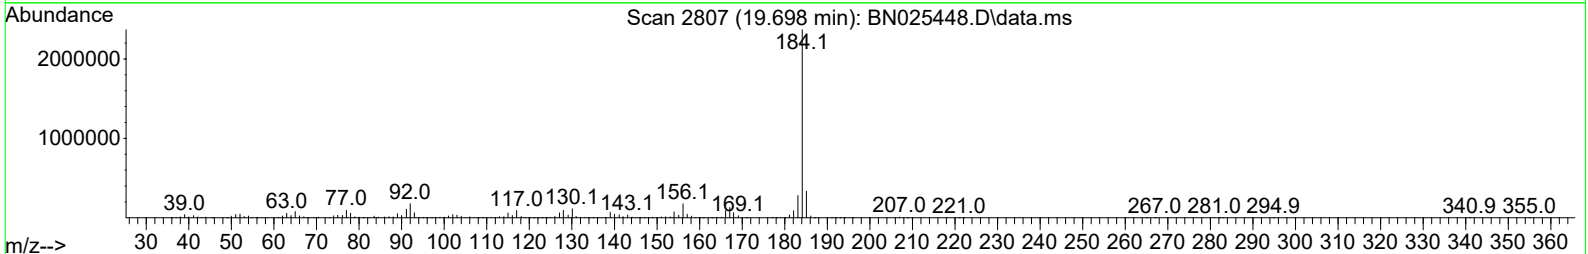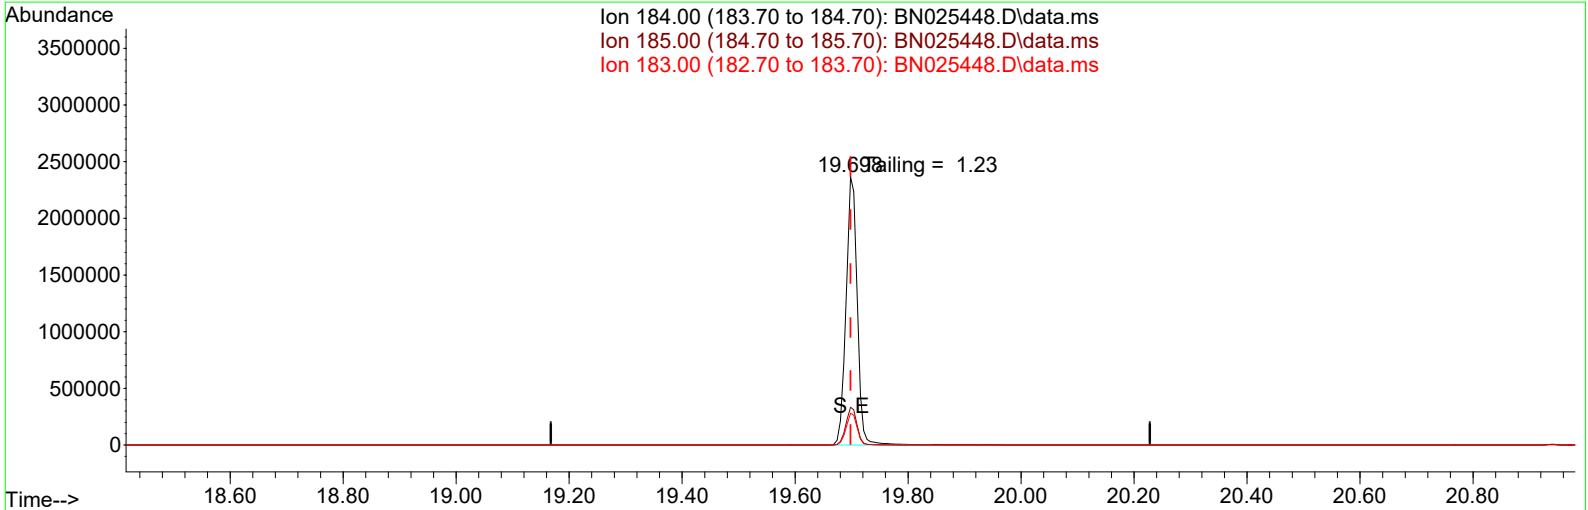

TIC: BN025448.D\data.ms

(77) Benzidine

19.698min ( 0.000) 0.00 ng

response 3276062

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.12
183.00	13.20	11.81
0.00	0.00	0.00