
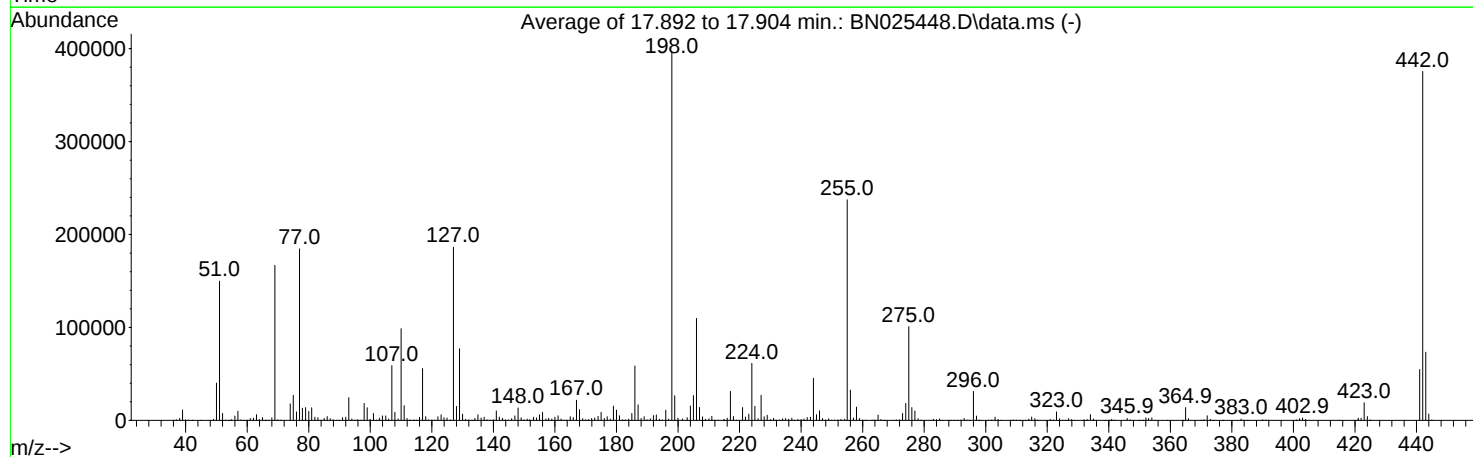


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051723\
Data File : BN025448.D
Acq On : 17 May 2023 09:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 18 03:36:39 2023

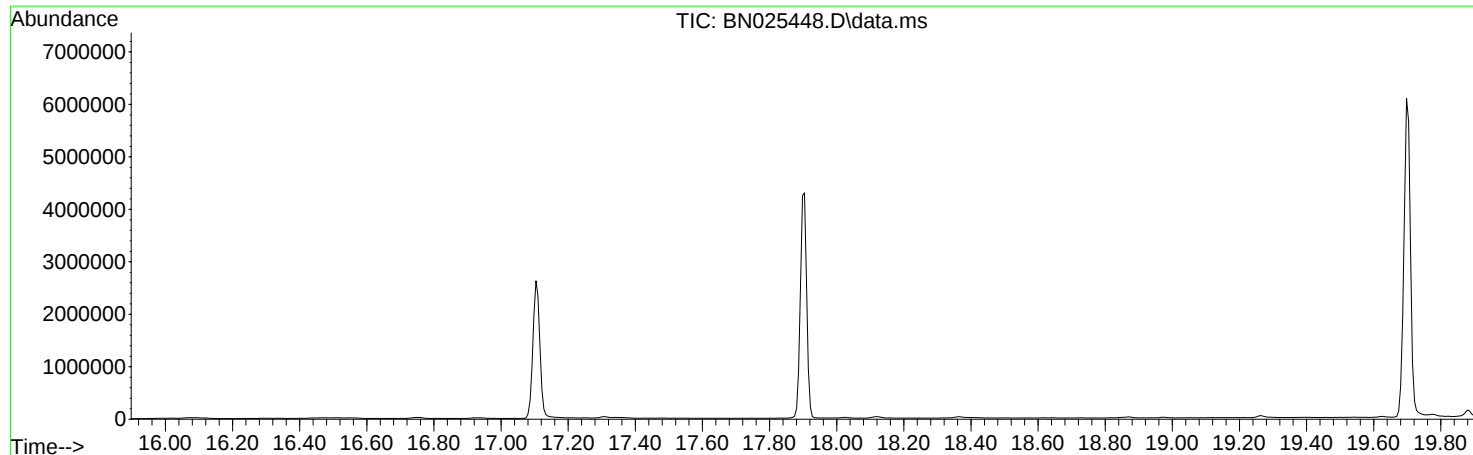

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	149829	PASS
68	69	0.00	2	1.6	2703	PASS
69	198	0.00	100	42.1	166824	PASS
70	69	0.00	2	0.5	769	PASS
127	198	10	80	47.1	186368	PASS
197	198	0.00	2	0.3	1322	PASS
198	198	100	100	100.0	395840	PASS
199	198	5	9	6.7	26485	PASS
275	198	10	60	25.5	100909	PASS
365	198	1	100	3.5	13759	PASS
441	198	0.01	100	13.8	54693	PASS
442	442	50	100	100.0	375488	PASS
443	442	15	24	19.5	73283	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/17/2023	BNA_N	<u>BN025448.D</u>
Compound Name	Response	Retention Time
DDT	1514168	20.939
DDD	15253	20.551
DDE	130	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15383	1529551	1.01

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051723\
Data File : BN025448.D
Acq On : 17 May 2023 09:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 18 05:36:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 05:36:50 2023
Response via : Initial Calibration

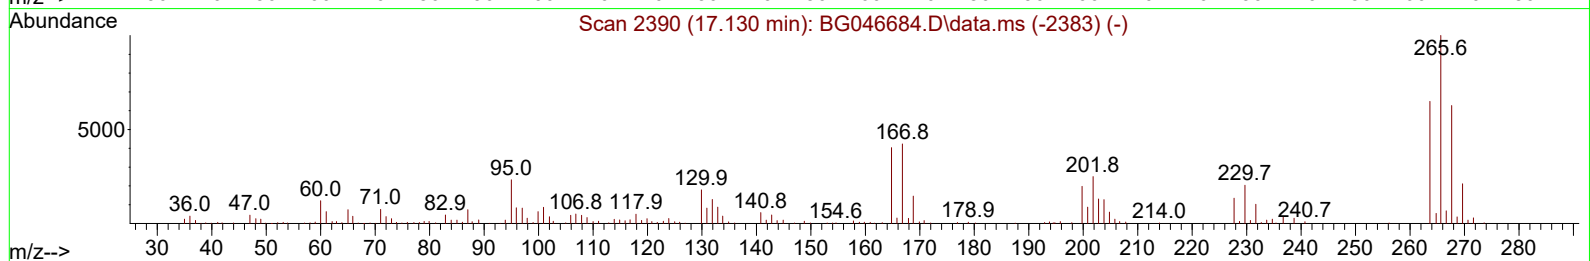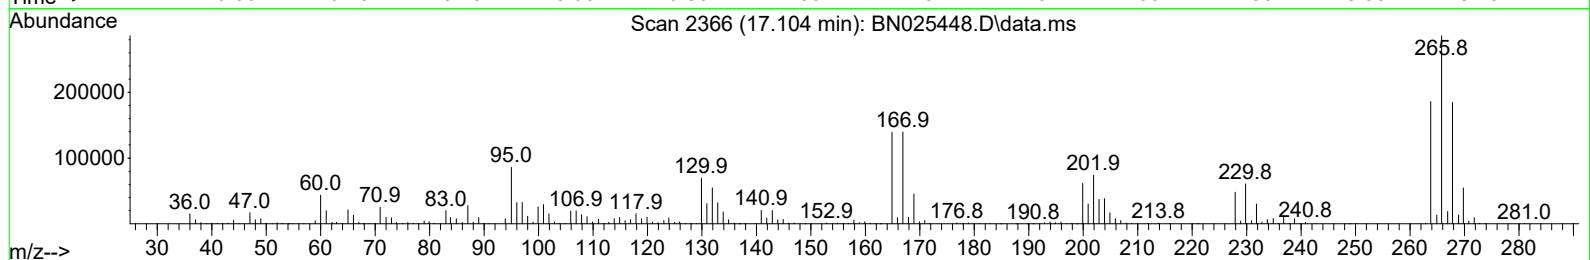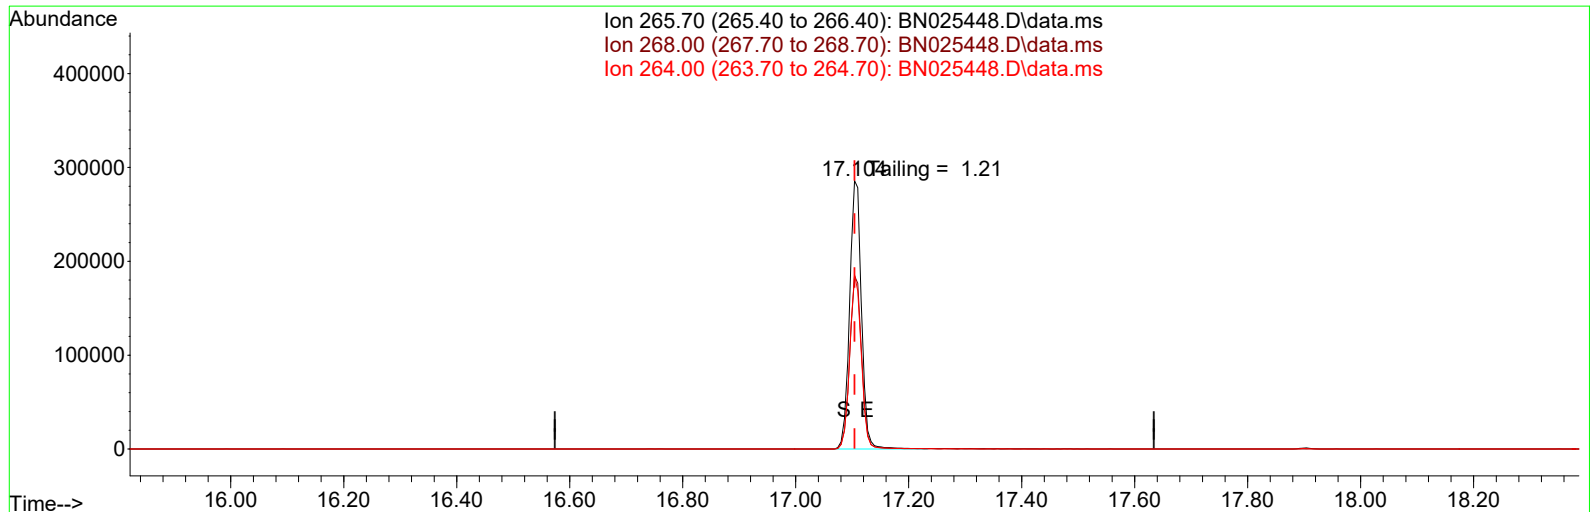

TIC: BN025448.D\data.ms

(70) Pentachlorophenol (C)

17.104min (0.000) 17533.93 ng




response 418585

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.50
264.00	61.60	64.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051723\
Data File : BN025448.D
Acq On : 17 May 2023 09:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 18 05:36:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 05:36:50 2023
Response via : Initial Calibration

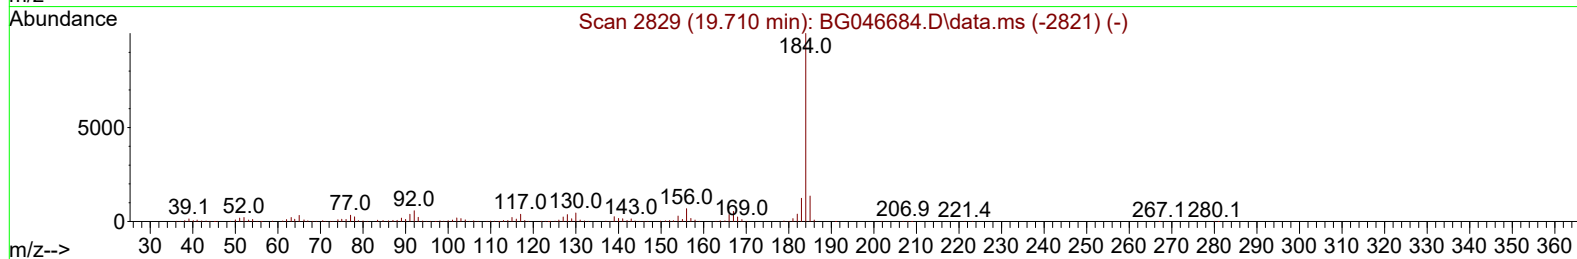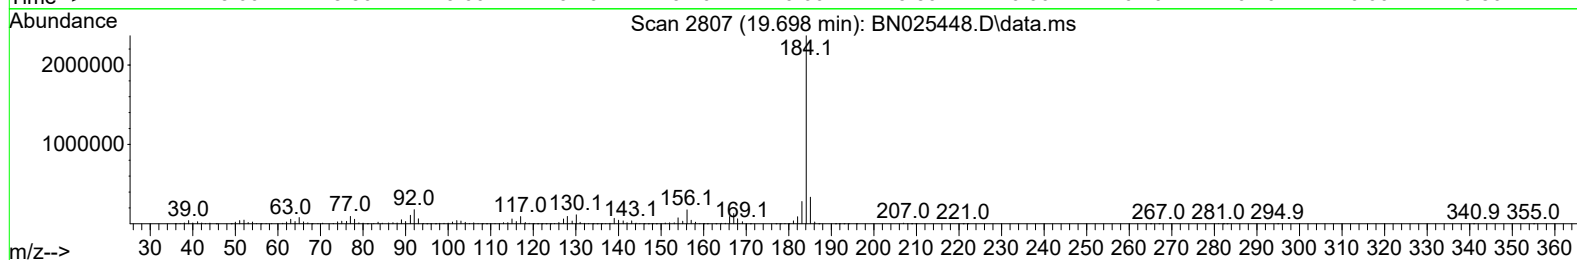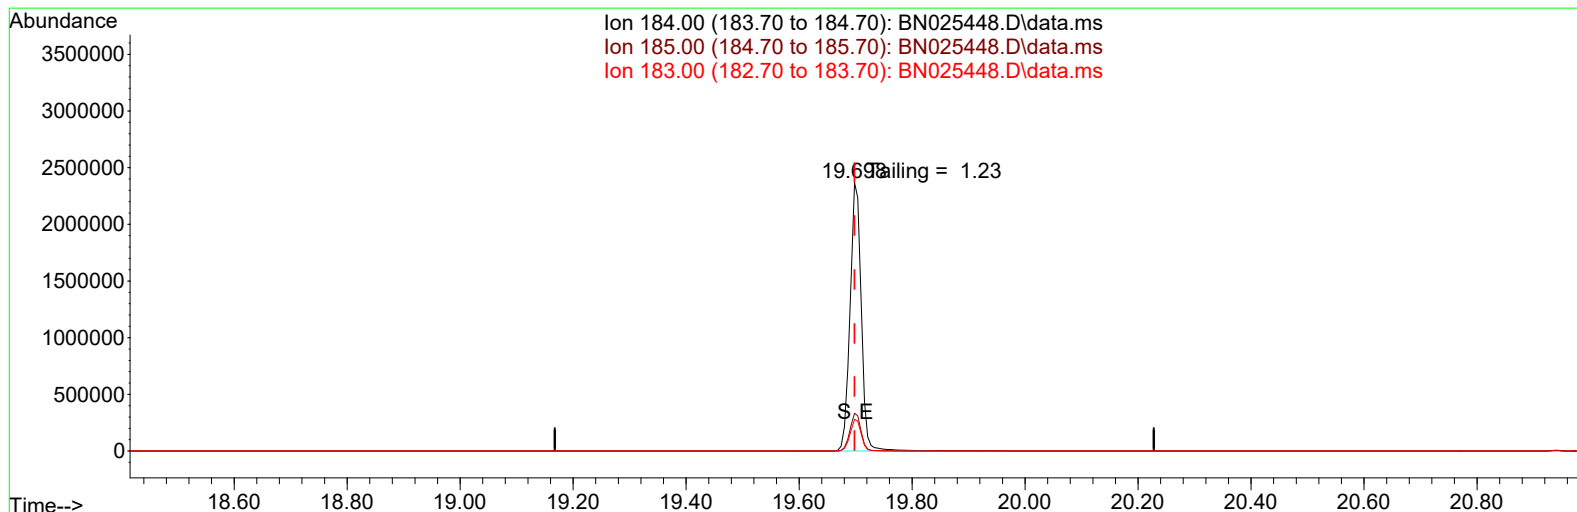

TIC: BN025448.D\data.ms

(77) Benzidine

19.698min (0.000) 0.00 ng

response 3276062

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.12
183.00	13.20	11.81
0.00	0.00	0.00