
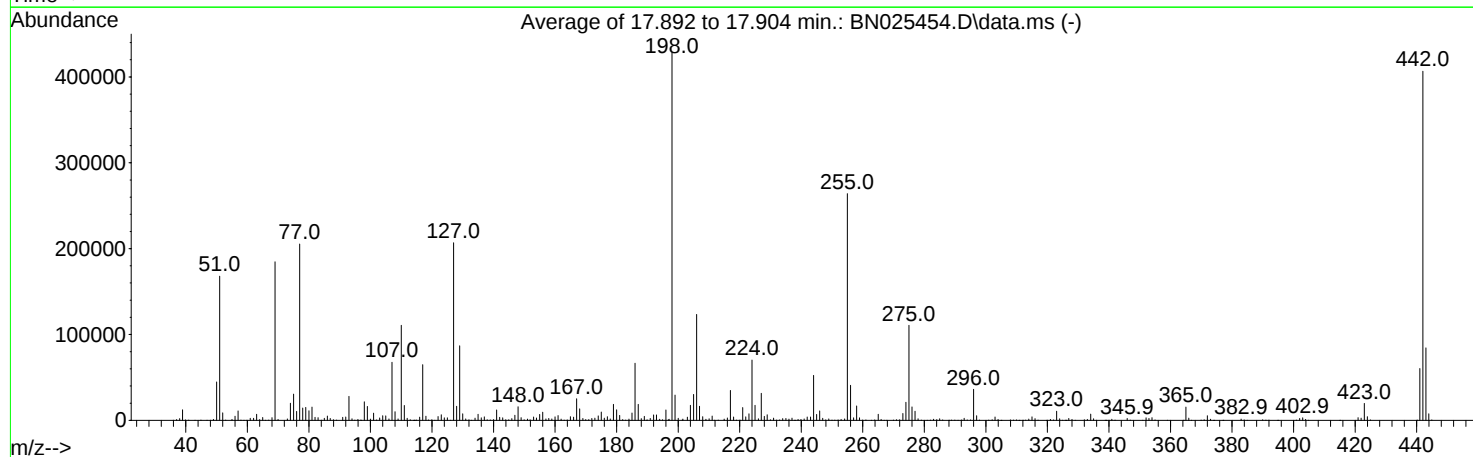


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051723\
 Data File : BN025454.D
 Acq On : 17 May 2023 15:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 18 03:36:39 2023

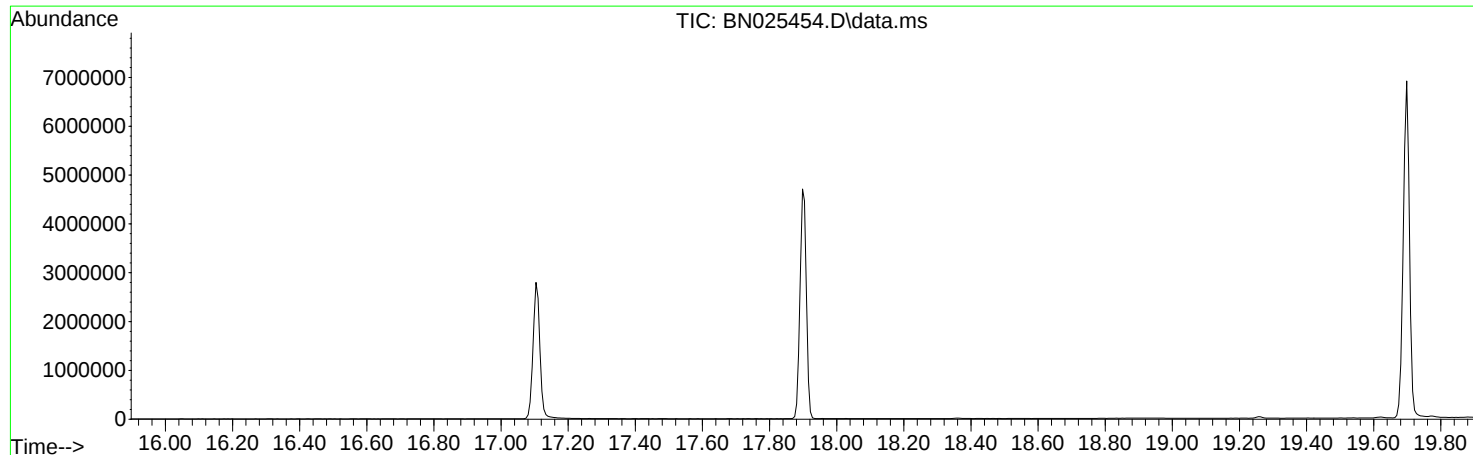

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	168000	PASS
68	69	0.00	2	1.7	3139	PASS
69	198	0.00	100	43.1	184619	PASS
70	69	0.00	2	0.6	1066	PASS
127	198	10	80	48.3	206848	PASS
197	198	0.00	2	0.3	1348	PASS
198	198	100	100	100.0	428459	PASS
199	198	5	9	6.9	29507	PASS
275	198	10	60	25.8	110677	PASS
365	198	1	100	3.6	15534	PASS
441	198	0.01	100	14.1	60317	PASS
442	442	50	100	100.0	406635	PASS
443	442	15	24	20.7	84339	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/17/2023	BNA_N	<u>BN025454.D</u>
Compound Name	Response	Retention Time
DDT	1628530	20.933
DDD	17163	20.545
DDE	94	19.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17257	1645787	1.05

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051723\
 Data File : BN025454.D
 Acq On : 17 May 2023 15:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 18 05:38:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 18 05:36:50 2023
 Response via : Initial Calibration

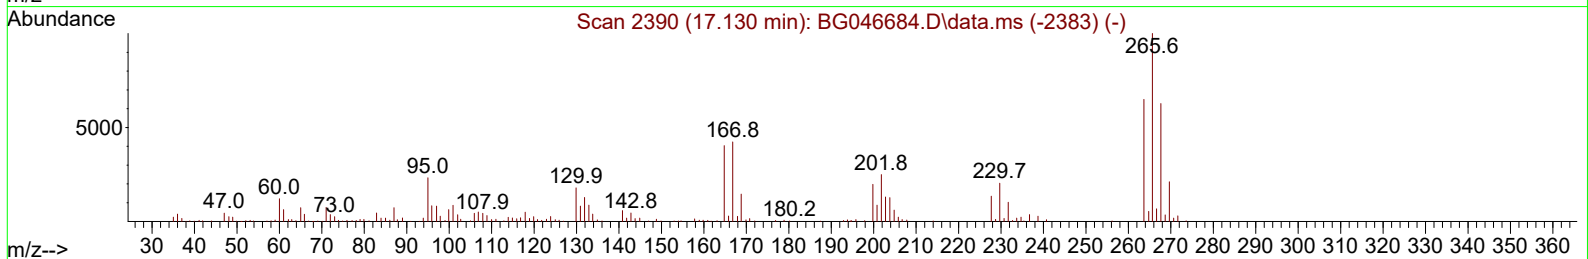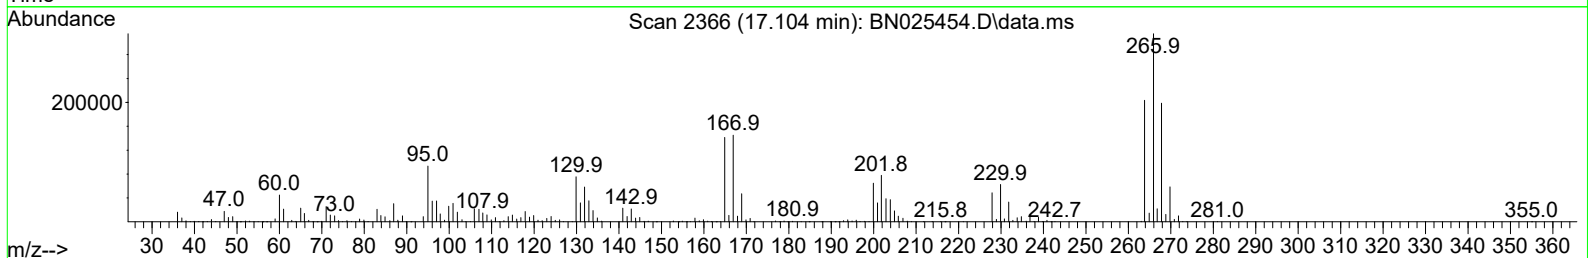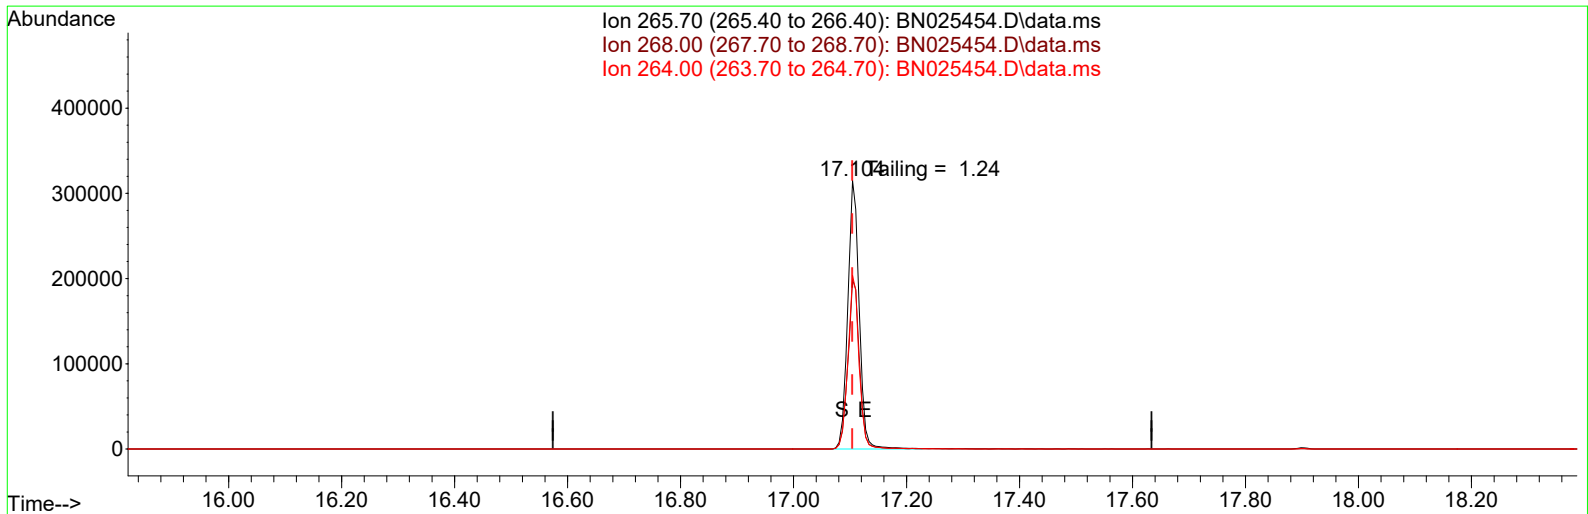

TIC: BN025454.D\data.ms

(70) Pentachlorophenol (C)

17.104min (+ 0.000) 17604.40 ng




response 443201

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.06
264.00	61.60	64.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051723\
Data File : BN025454.D
Acq On : 17 May 2023 15:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 18 05:38:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 05:36:50 2023
Response via : Initial Calibration

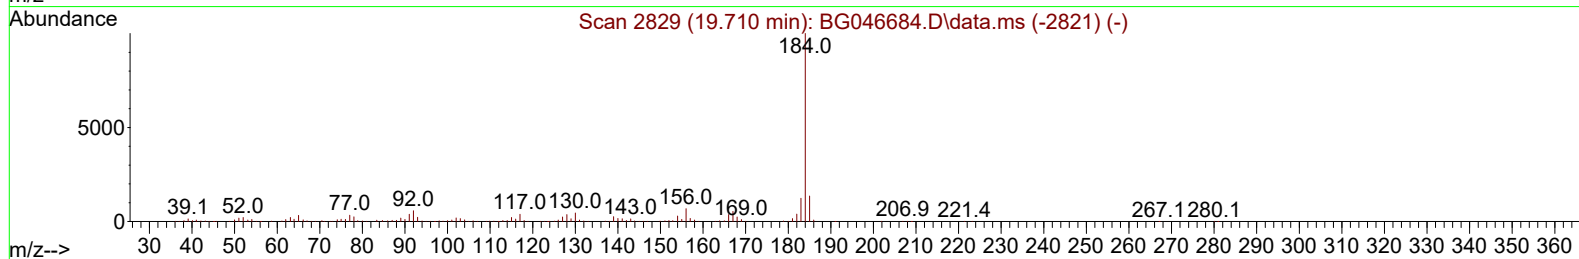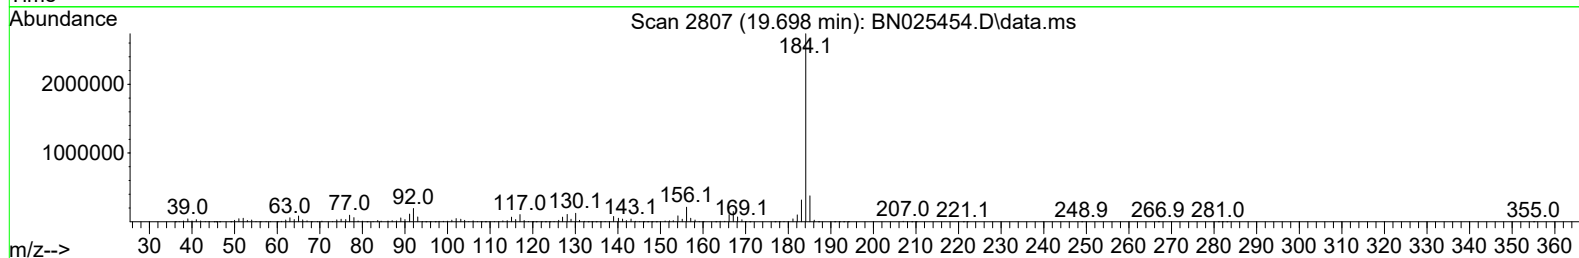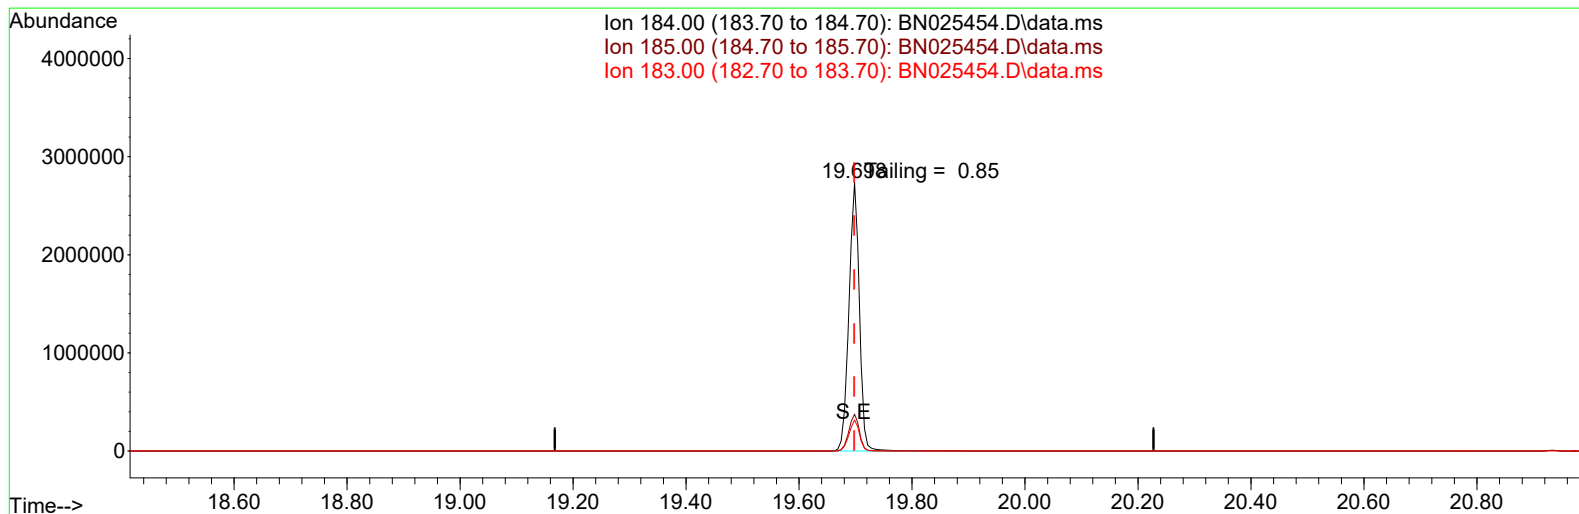

TIC: BN025454.D\data.ms

(77) Benzidine

19.698min (+ 0.000) 0.00 ng

response 3522720

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.77
183.00	13.20	11.57
0.00	0.00	0.00