




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051724\
Data File : BN031553.D
Acq On : 16 May 2024 16:52
Operator : MA/JU
Sample : PB160730BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK730

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/17/2024
Supervised By :mohammad ahmed 05/18/2024

Quant Time: May 16 17:21:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN051624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 12:57:23 2024
Response via : Initial Calibration

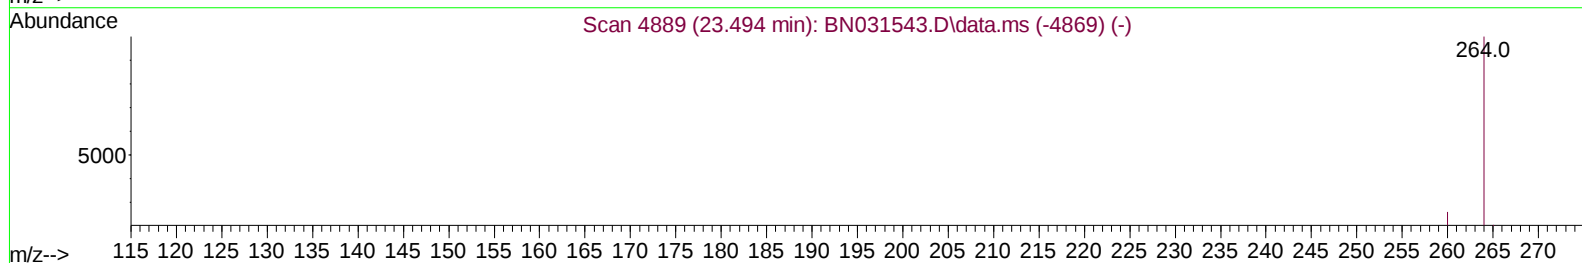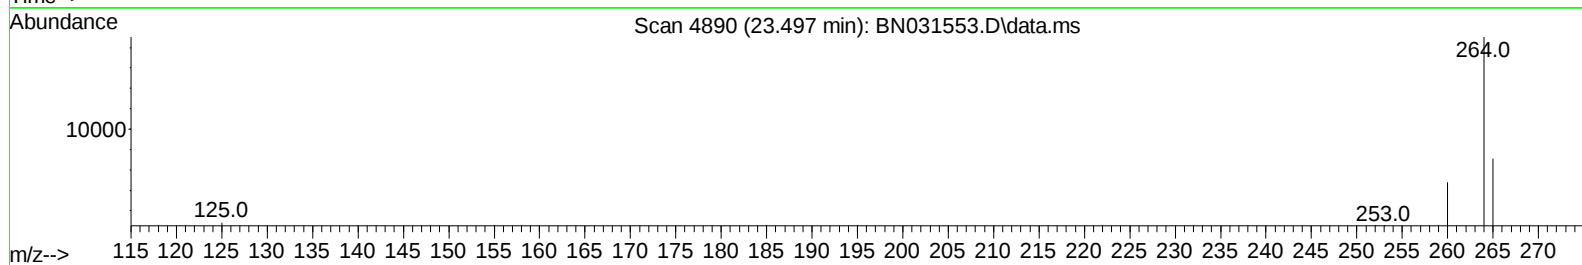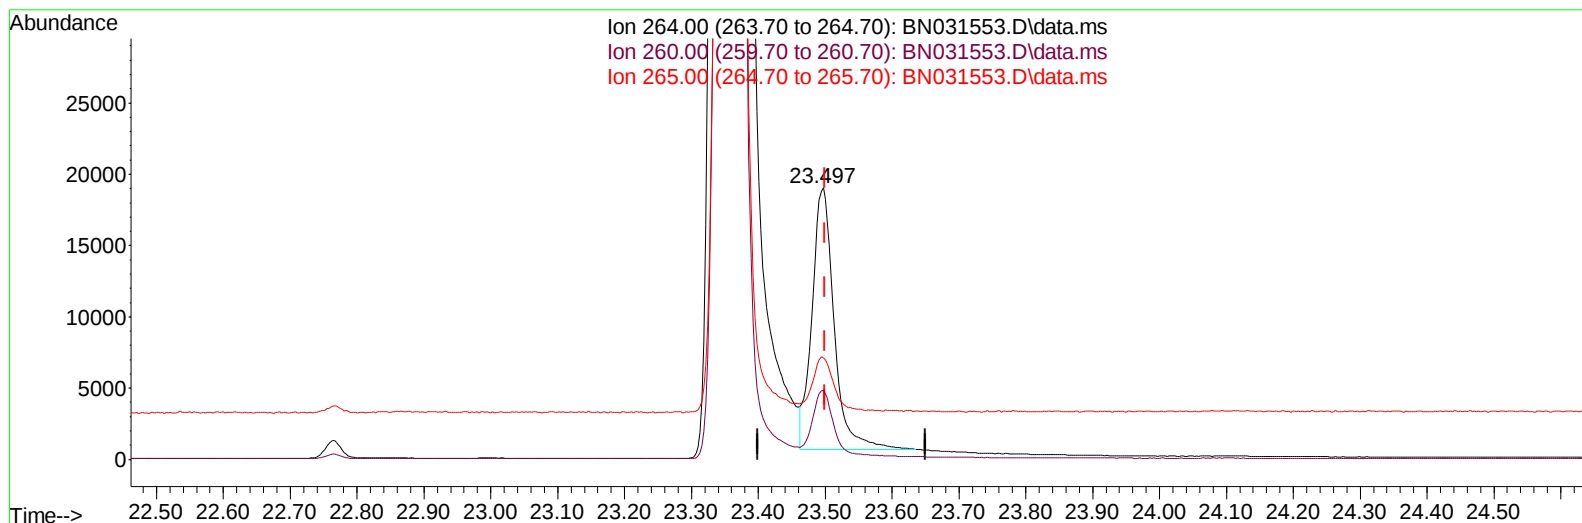

TIC: BN031553.D\data.ms

(23) Perylene-d12 (I)

23.497min (-0.003) 0.40 ng/u1

response 41894

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	25.28
265.00	44.70	37.39
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051724\
Data File : BN031553.D
Acq On : 16 May 2024 16:52
Operator : MA/JU
Sample : PB160730BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK730

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/17/2024
Supervised By :mohammad ahmed 05/18/2024

Quant Time: May 16 17:21:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN051624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 12:57:23 2024
Response via : Initial Calibration

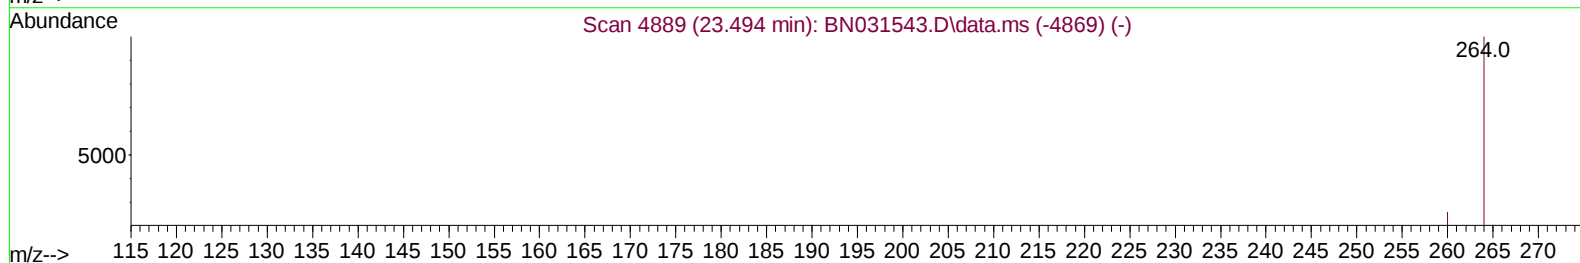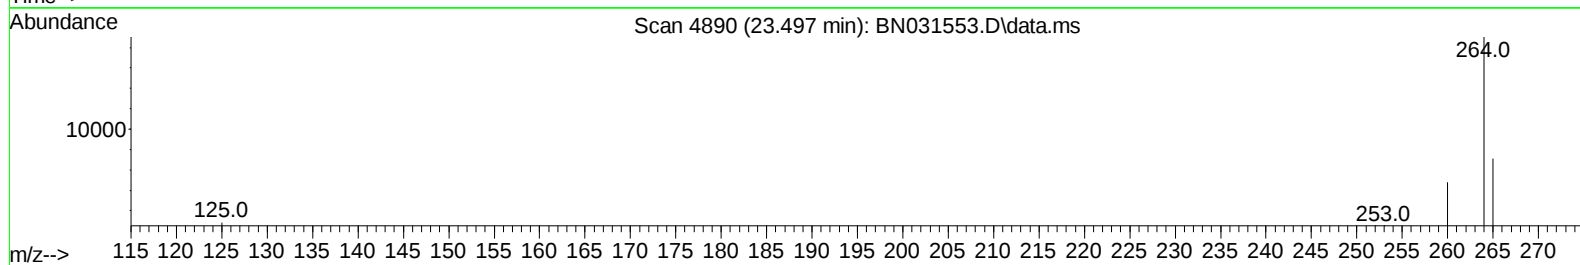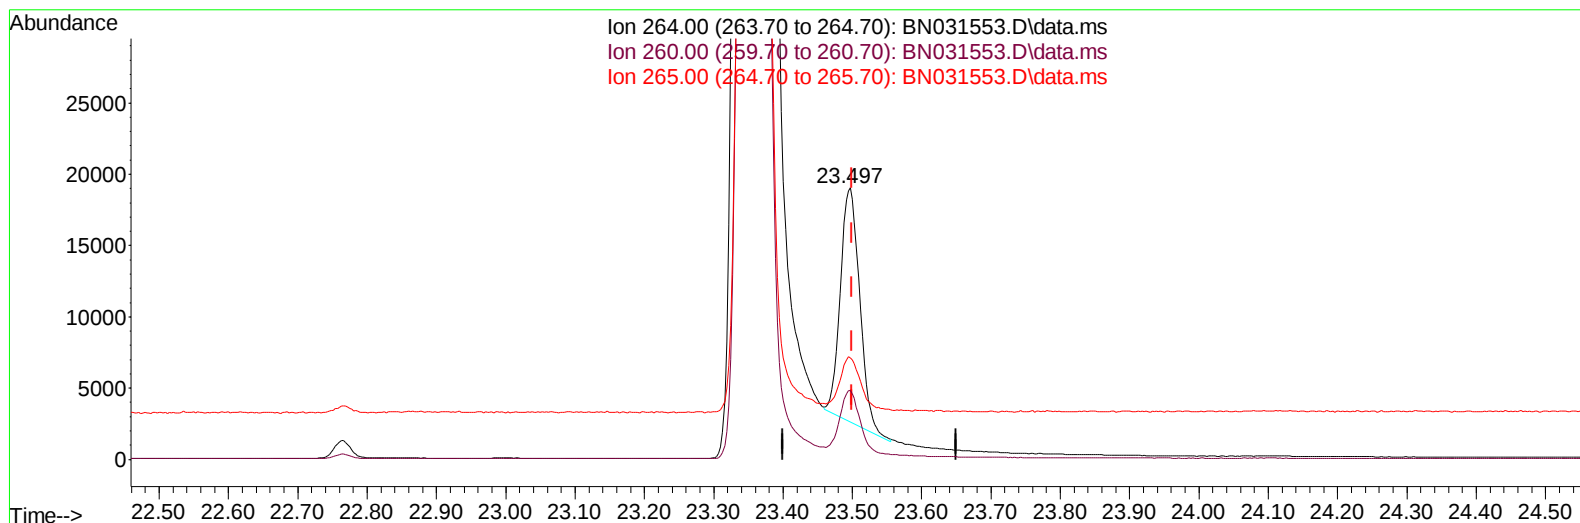

TIC: BN031553.D\data.ms

(23) Perylene-d12 (I)

23.497min (-0.003) 0.40 ng/ul m

response 31529

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	25.28
265.00	44.70	37.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051724\
 Data File : BN031553.D
 Acq On : 16 May 2024 16:52
 Operator : MA/JU
 Sample : PB160730BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK730

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/17/2024
 Supervised By :mohammad ahmed 05/18/2024

Quant Time: May 16 17:21:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN051624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 15 12:57:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.700	152	14927	0.400	ng/ul	0.00
4) Naphthalene-d8	10.481	136	50624	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.336	164	27393	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.075	188	61867	0.400	ng/ul	0.00
17) Chrysene-d12	21.261	240	42689	0.400	ng/ul	0.00
23) Perylene-d12	23.497	264	31529m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	76220	4.238	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.076	152	16713	0.233	ng/ul	0.00
18) Fluoranthene-d10	19.106	212	34975	0.295	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051724\
Data File : BN031553.D
Acq On : 16 May 2024 16:52
Operator : MA/JU
Sample : PB160730BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK730

Manual IntegrationsAPPROVED

Quant Time: May 16 17:21:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN051624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 12:57:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2024
Supervised By :mohammad ahmed 05/18/2024

