
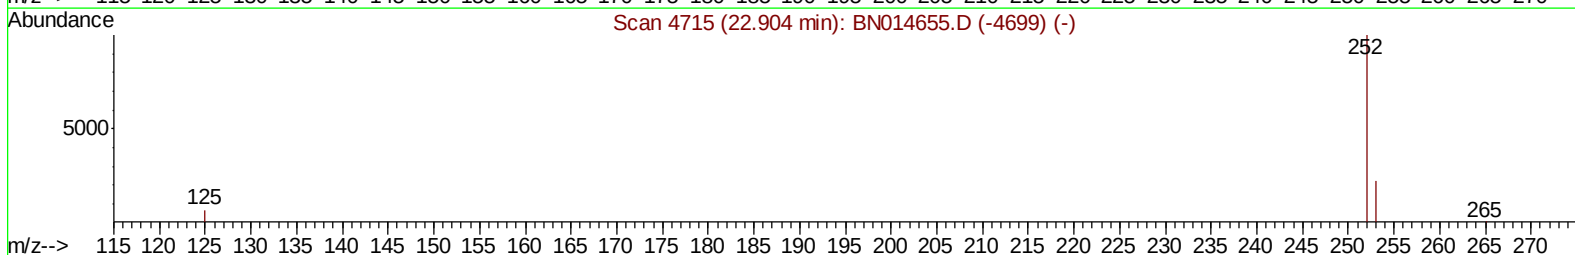
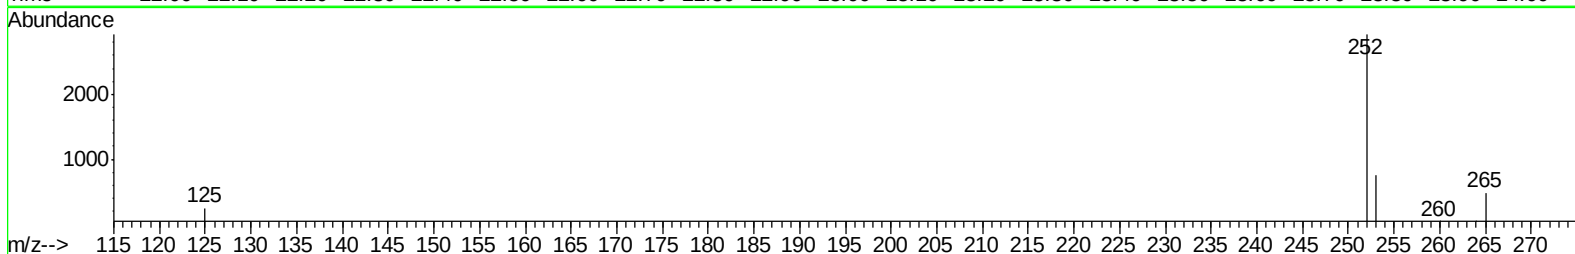


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051821\
Data File : BN014664.D
Acq On : 18 May 2021 13:52
Operator : CG/JU
Sample : M2402-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: May 18 17:29:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 15:50:11 2021
Response via : Initial Calibration

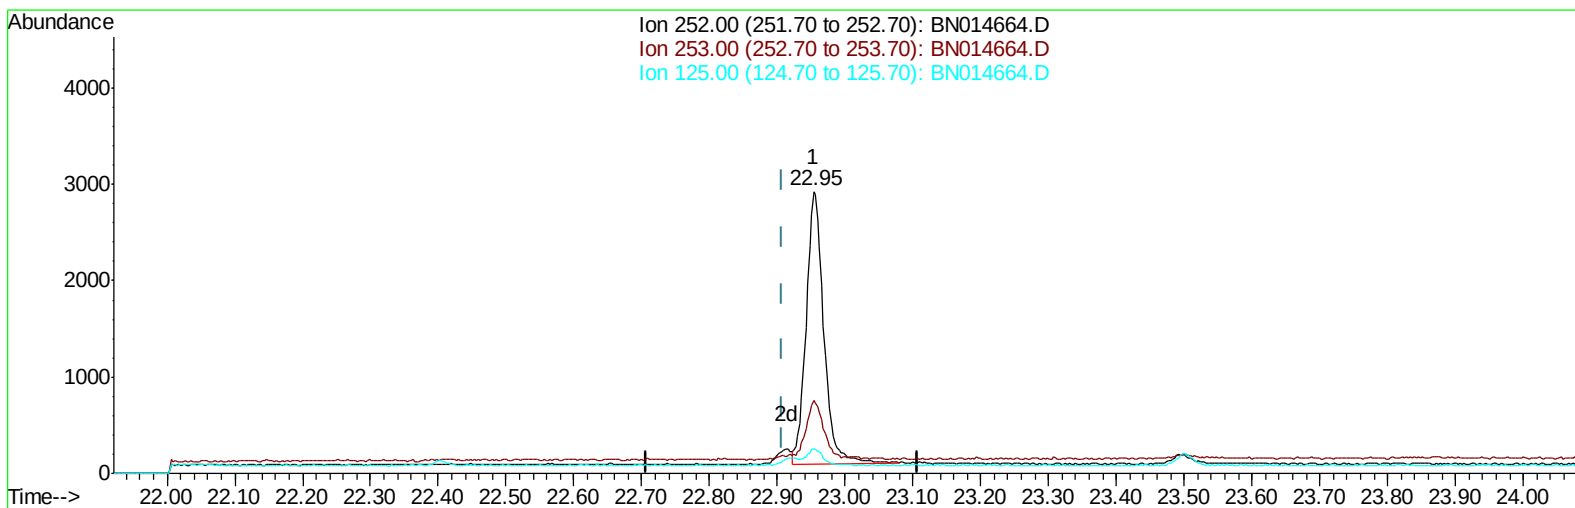

TIC: BN014664.D

(24) Benzo(b)fluoranthene

22.954min (+0.046) 0.40ng/ul

response 5107

Ion	Exp%	Act%
252.00	100	100
253.00	25.10	25.80
125.00	9.70	8.52
0.00	0.00	0.00