

Quantitation Report (QT Reviewed)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051821\
 Data File : BN014669.D
 Acq On : 18 May 2021 18:24
 Operator : CG/JU
 Sample : M2445-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG1Z4

Manual Integrations
 APPROVED

mohammad
 5/19/2021 11:39:19 AM

Quant Time: May 19 08:19:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 15:50:11 2021
 Response via : Initial Calibration

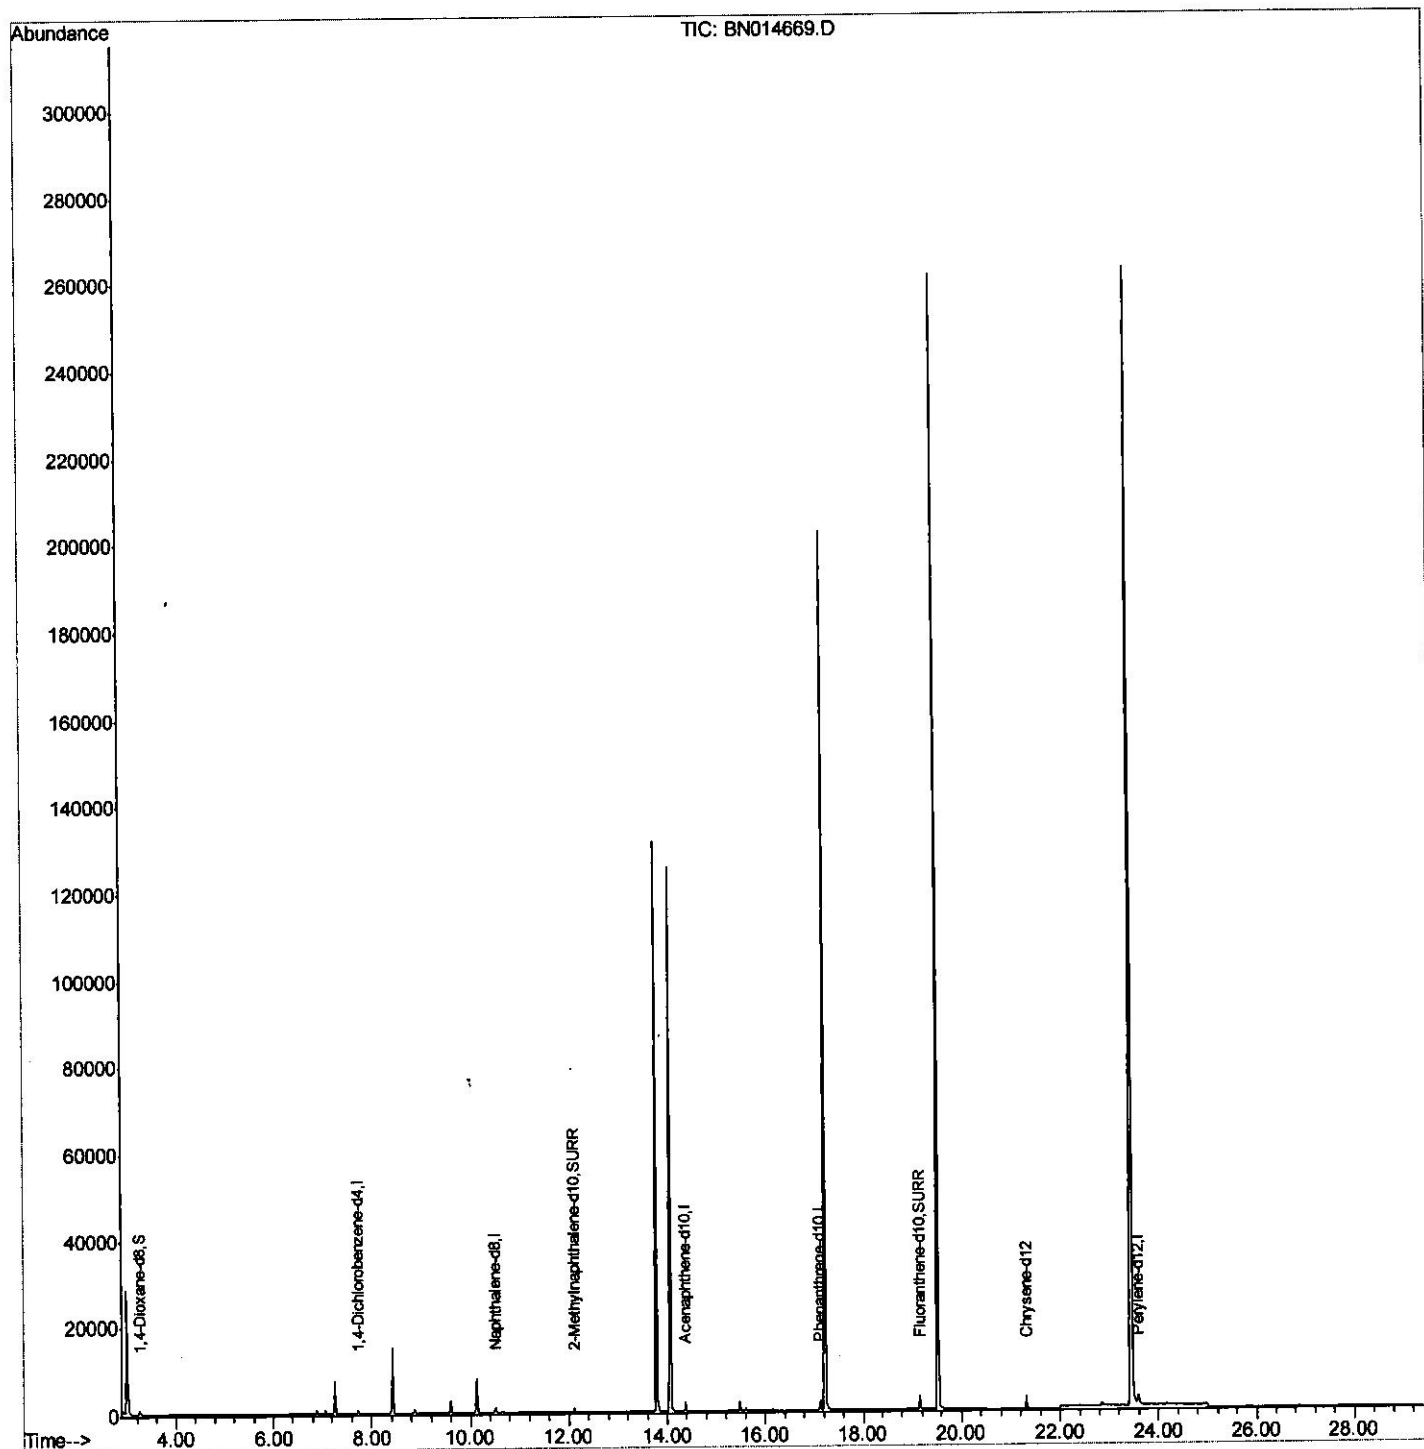

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051821\
 Data File : BN014669.D
 Acq On : 18 May 2021 18:24
 Operator : CG/JU
 Sample : M2445-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG1Z4

Quant Time: May 19 02:51:06 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 15:50:11 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 5/19/2021 11:39:19 AM

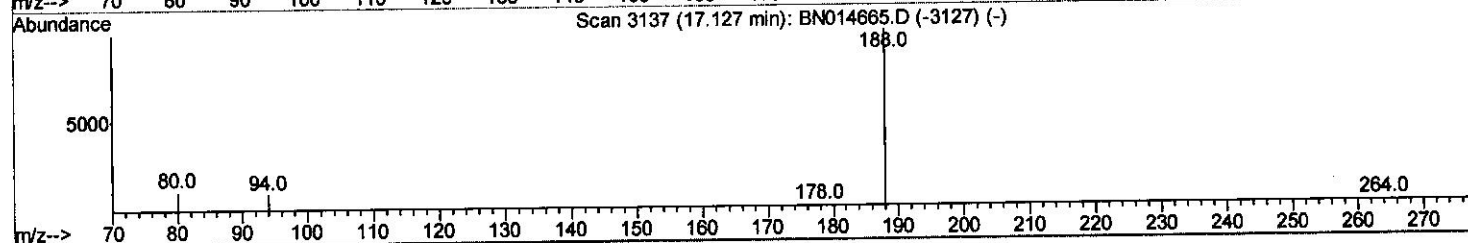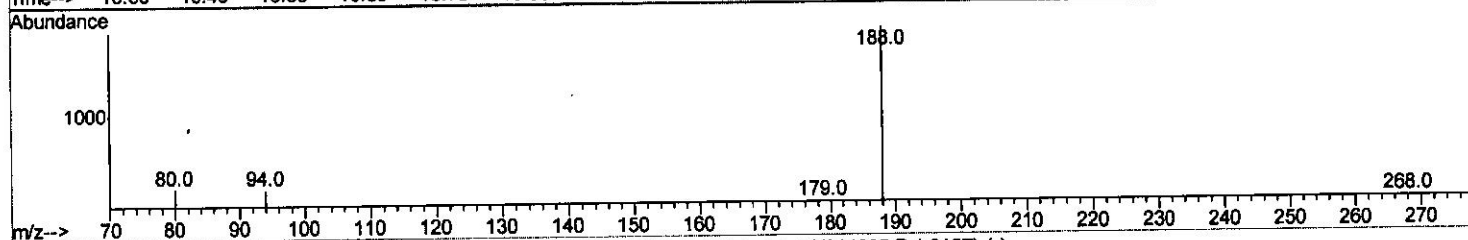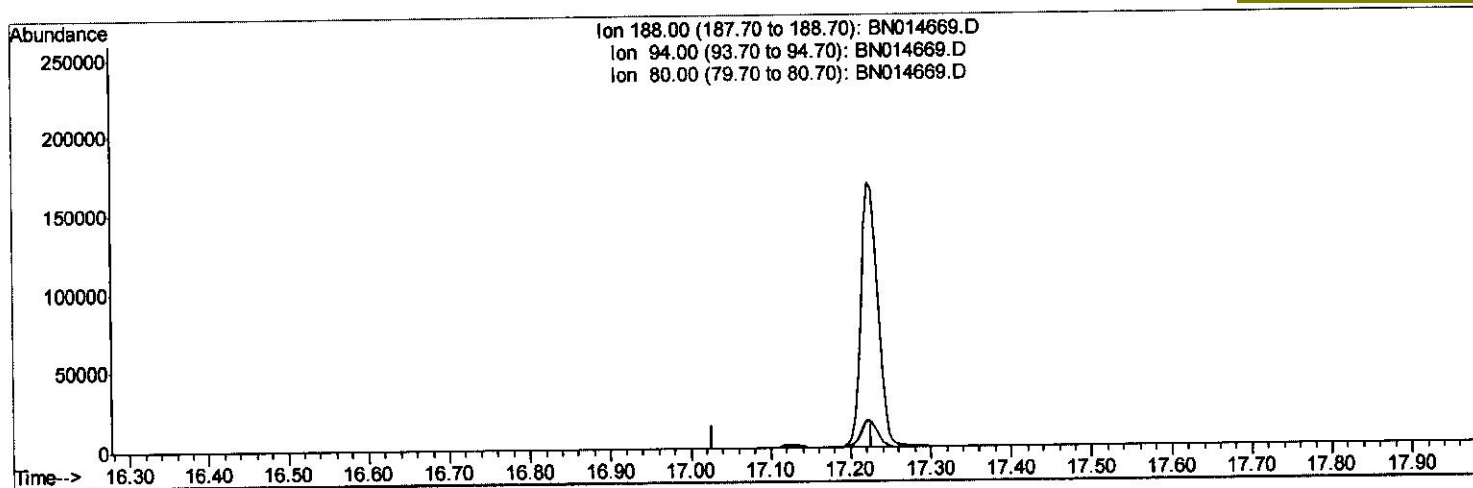

TIC: BN014669.D

(13) Phenanthrene-d10 (l)

17.127min (-17.127) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.10	0.00#
80.00	12.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051821\
 Data File : BN014669.D
 Acq On : 18 May 2021 18:24
 Operator : CG/JU
 Sample : M2445-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG1Z4

Manual Integrations
 APPROVED

mohammad
 5/19/2021 11:39:19 AM

Quant Time: May 19 02:51:06 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 15:50:11 2021
 Response via : Initial Calibration

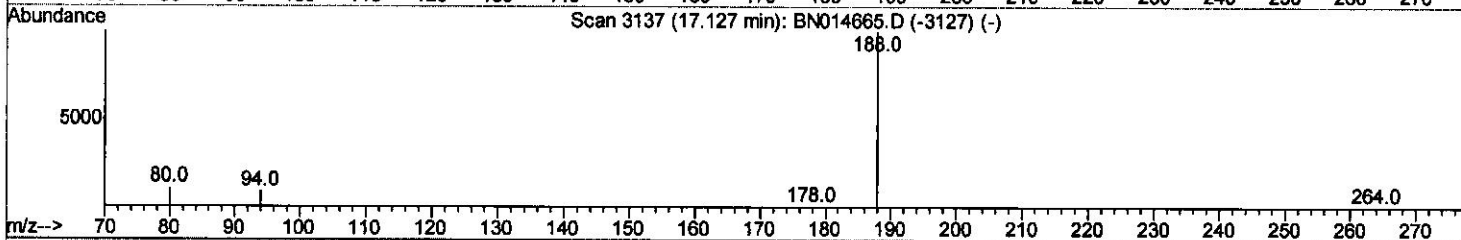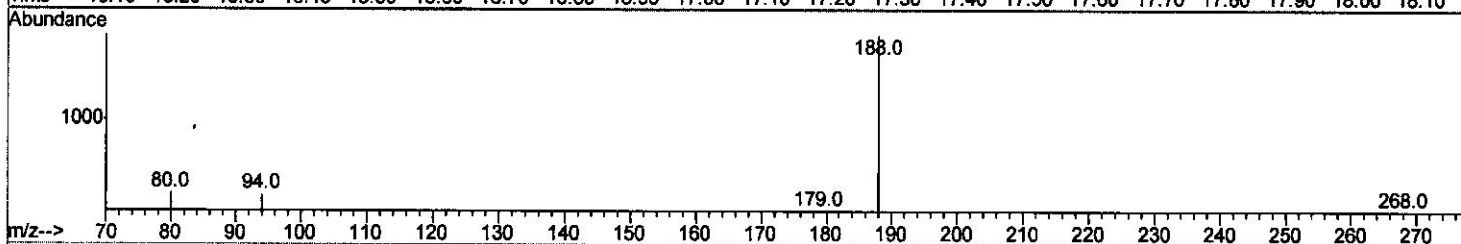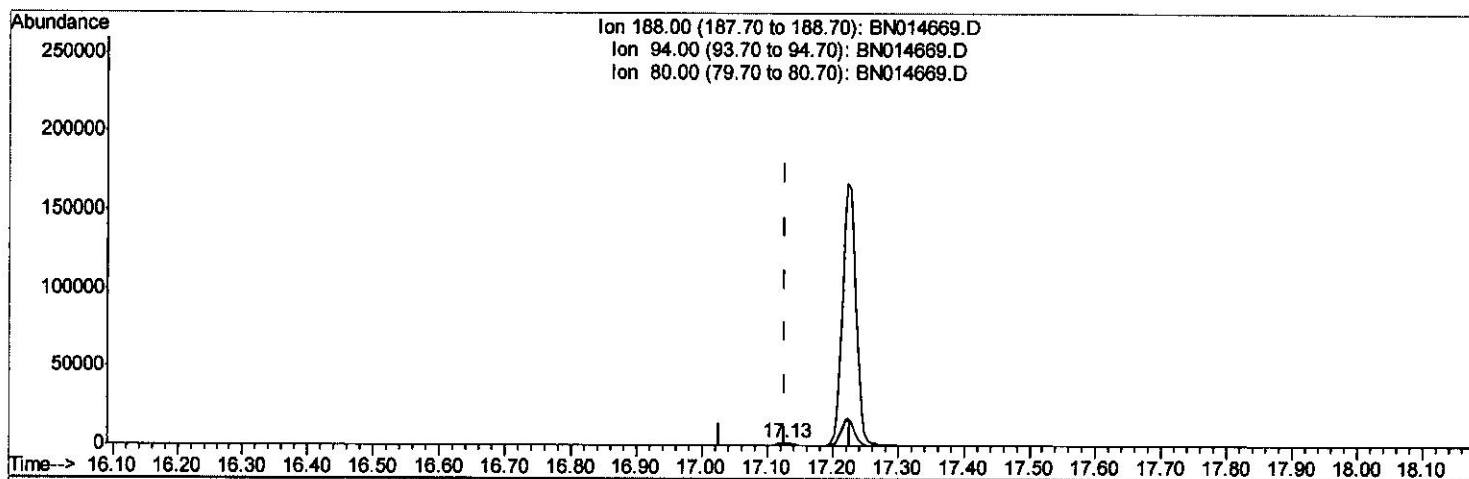

TIC: BN014669.D

(13) Phenanthrene-d10 (I)

17.126min (-0.001) 0.40ng/ul m

response 2598

Ion	Exp%	Act%
188.00	100	100
94.00	11.10	11.33
80.00	12.50	12.12
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051821\
 Data File : BN014669.D
 Acq On : 18 May 2021 18:24
 Operator : CG/JU
 Sample : M2445-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG1Z4

Quant Time: May 19 08:19:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 15:50:11 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 5/19/2021 11:39:19 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	440	0.40	ng/ul	0.00
4) Naphthalene-d8	10.51	136	1456	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.37	164	1136	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.13	188	2598m	0.40	ng/ul	0.00
17) Chrysene-d12	21.33	240	2869	0.40	ng/ul	0.00
23) Perylene-d12	23.59	264	3230	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	626	1.39	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.11	152	978	0.39	ng/ul	0.00
18) Fluoranthene-d10	19.16	212	3677	0.51	ng/ul	0.00

11/19/21 JU

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed