
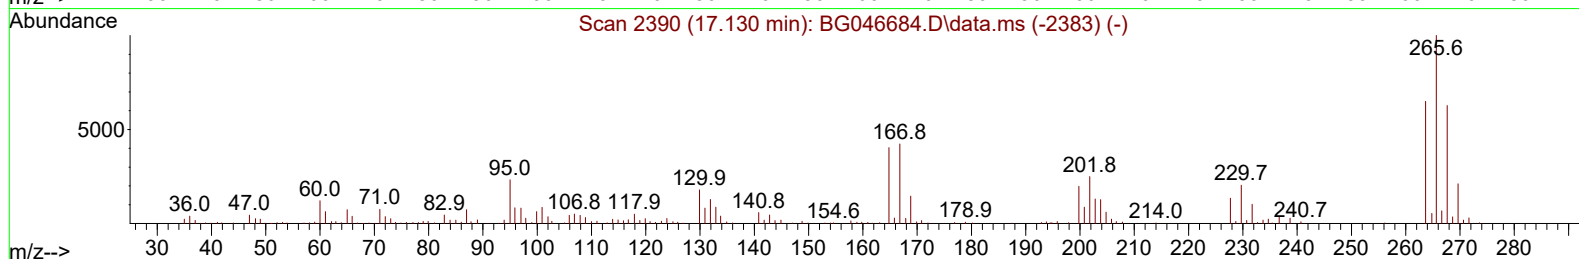
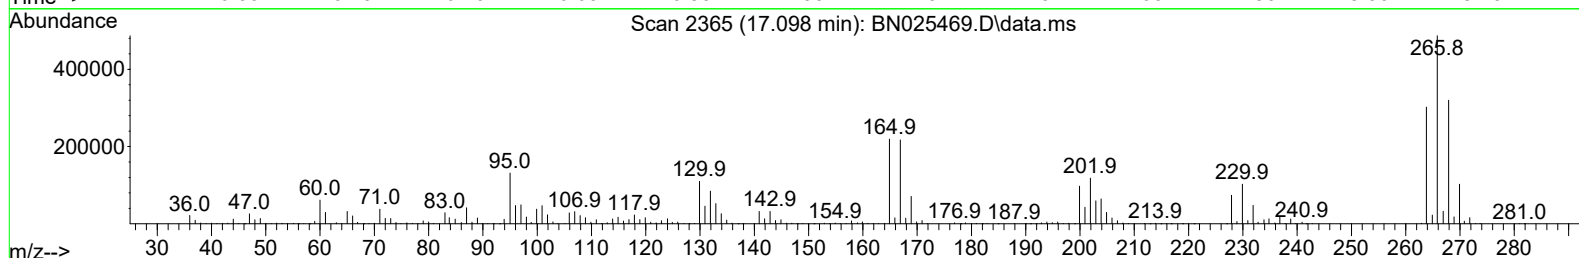


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051823\
Data File : BN025469.D
Acq On : 18 May 2023 11:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 05:57:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 19 05:57:12 2023
Response via : Initial Calibration

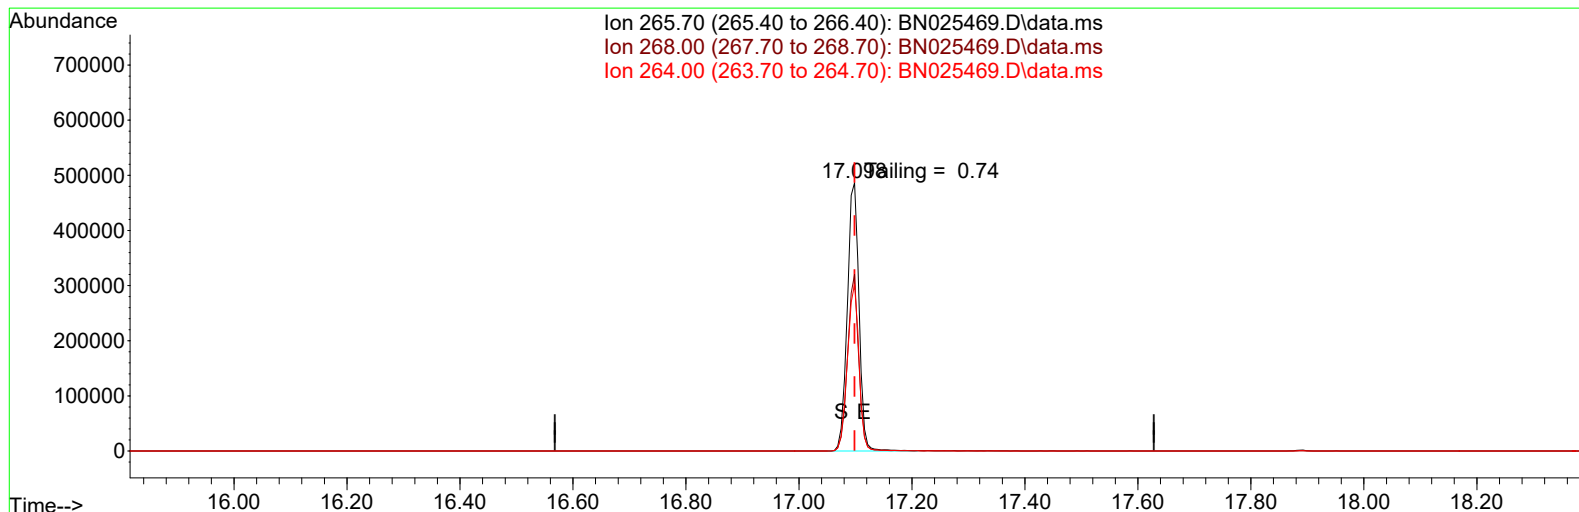

TIC: BN025469.D\data.ms

(70) Pentachlorophenol (C)




17.098min (0.000) 21655.13 ng

response 701189

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.74
264.00	61.60	62.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051823\
 Data File : BN025469.D
 Acq On : 18 May 2023 11:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 05:57:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 19 05:57:12 2023
 Response via : Initial Calibration

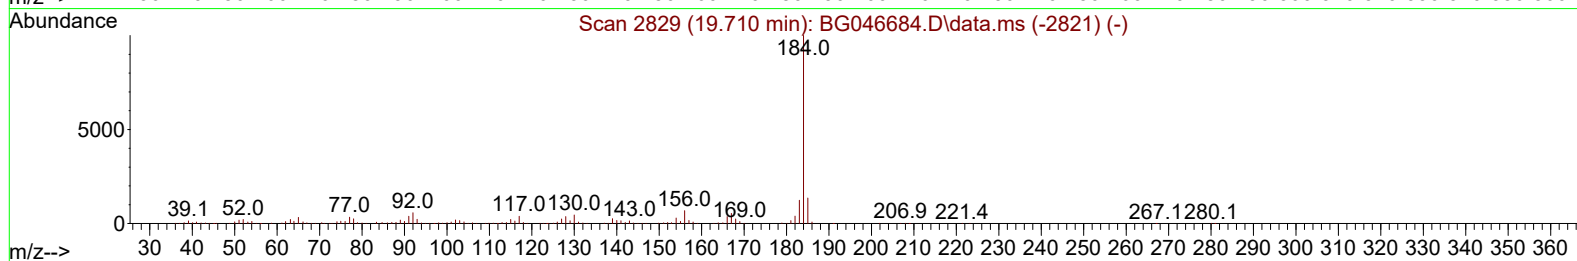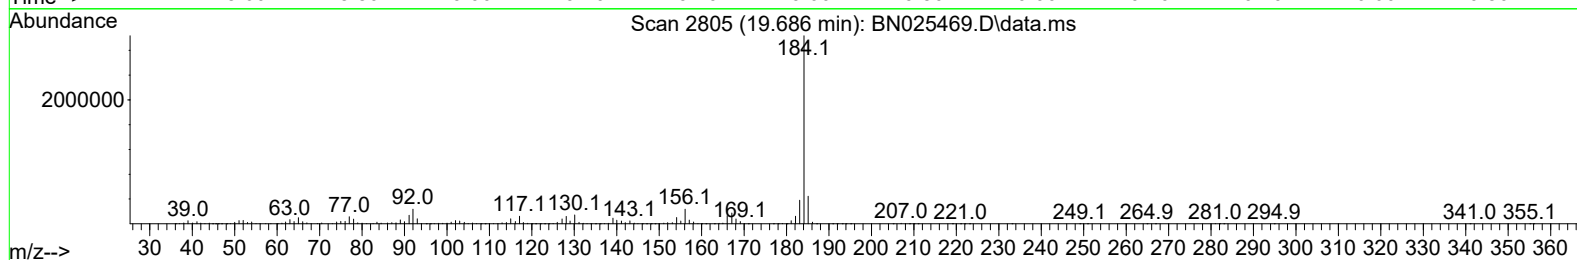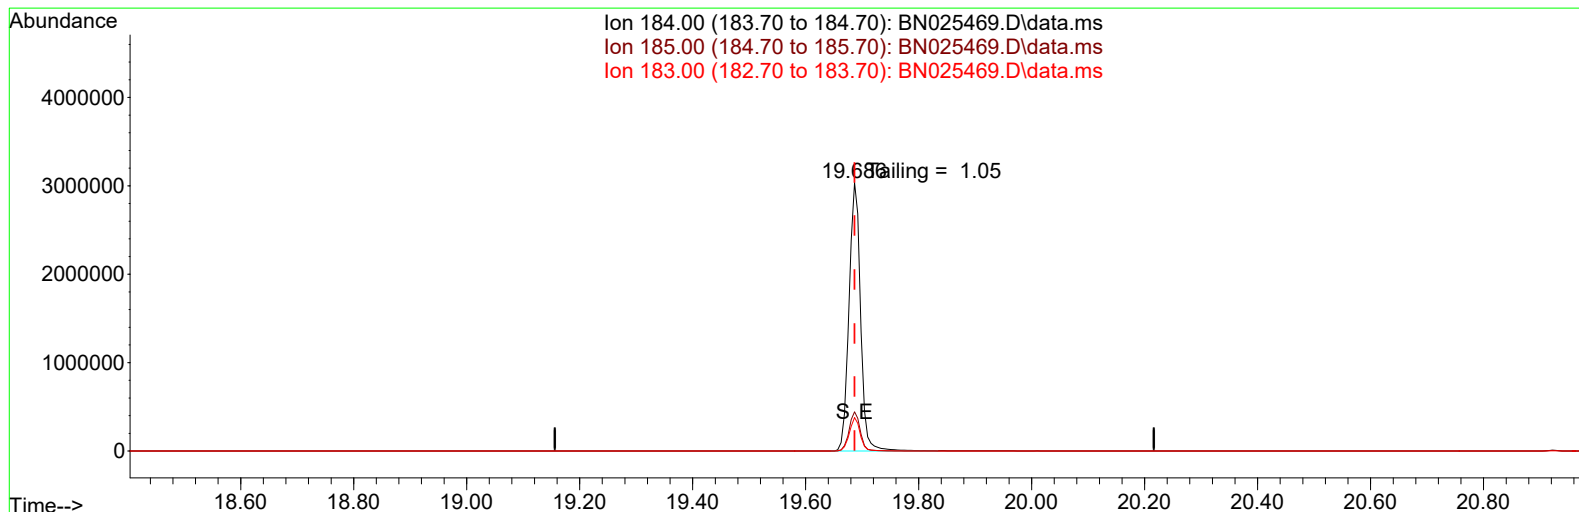

TIC: BN025469.D\data.ms

(77) Benzidine

19.686min (0.000) 2595362.65 ng

response 4320163

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.62
183.00	13.20	12.51
0.00	0.00	0.00