
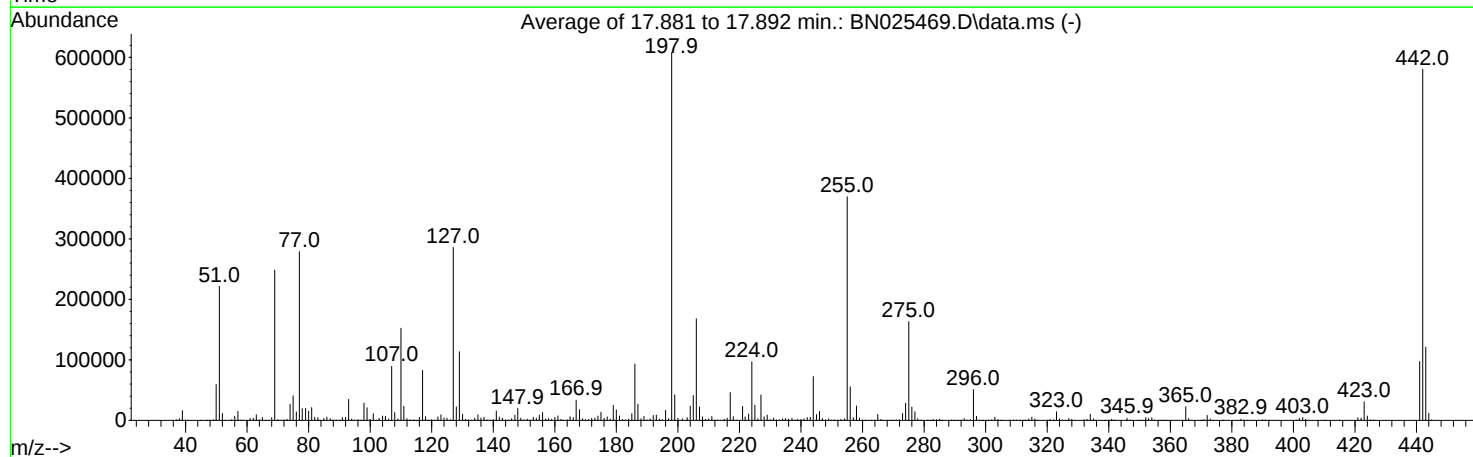


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051823\
 Data File : BN025469.D
 Acq On : 18 May 2023 11:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 19 02:17:42 2023

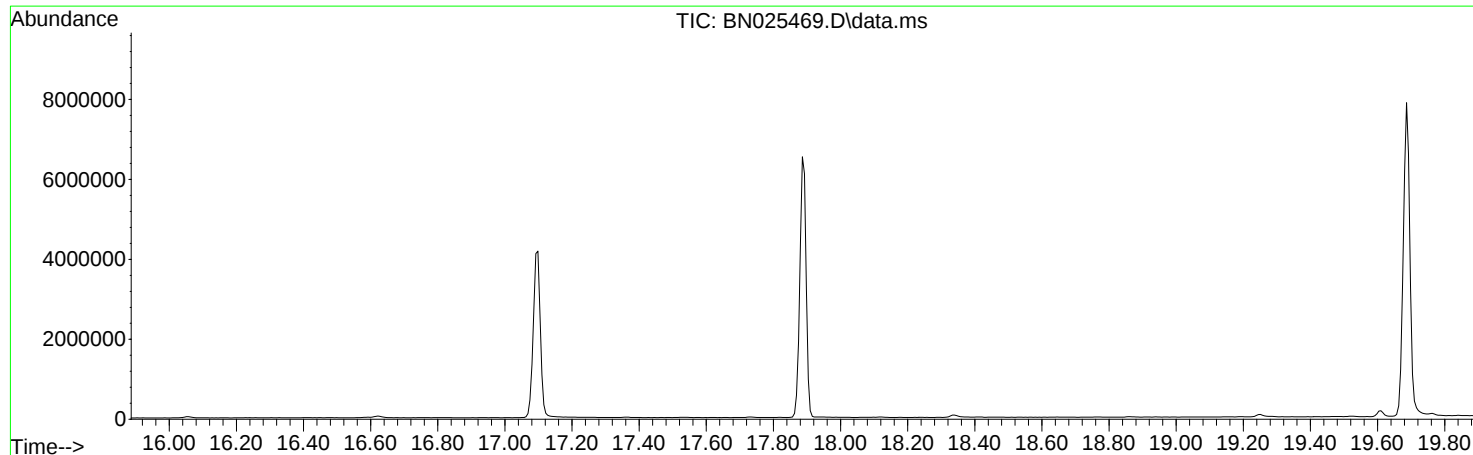

AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	221301	PASS
68	69	0.00	2	1.8	4414	PASS
69	198	0.00	100	40.8	248389	PASS
70	69	0.00	2	0.5	1254	PASS
127	198	10	80	47.0	285908	PASS
197	198	0.00	2	0.5	2962	PASS
198	198	100	100	100.0	608064	PASS
199	198	5	9	7.0	42261	PASS
275	198	10	60	26.8	163104	PASS
365	198	1	100	3.7	22564	PASS
441	198	0.01	100	16.0	97347	PASS
442	442	50	100	100.0	580160	PASS
443	442	15	24	20.9	121269	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/18/2023	BNA_N	<u>BN025469.D</u>
Compound Name	Response	Retention Time
DDT	2170021	20.927
DDD	22706	20.533
DDE	173	19.969
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22879	2192900	1.04

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051823\
 Data File : BN025469.D
 Acq On : 18 May 2023 11:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 19 05:57:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 19 05:57:12 2023
 Response via : Initial Calibration

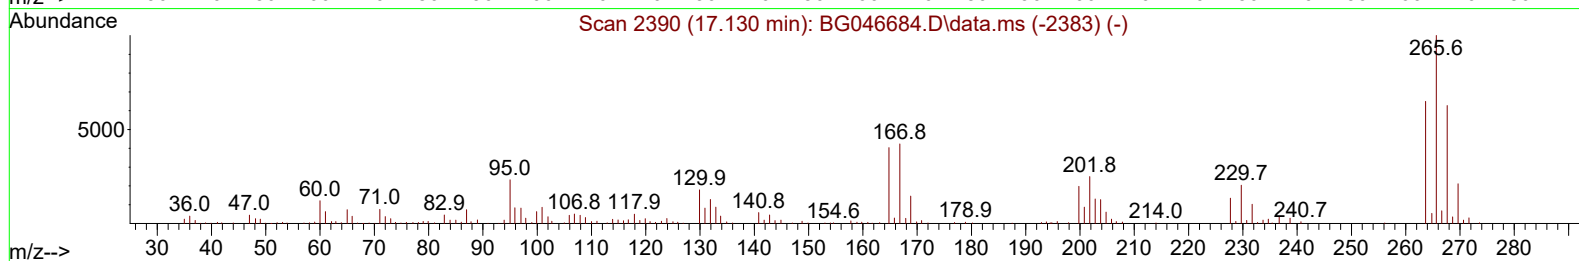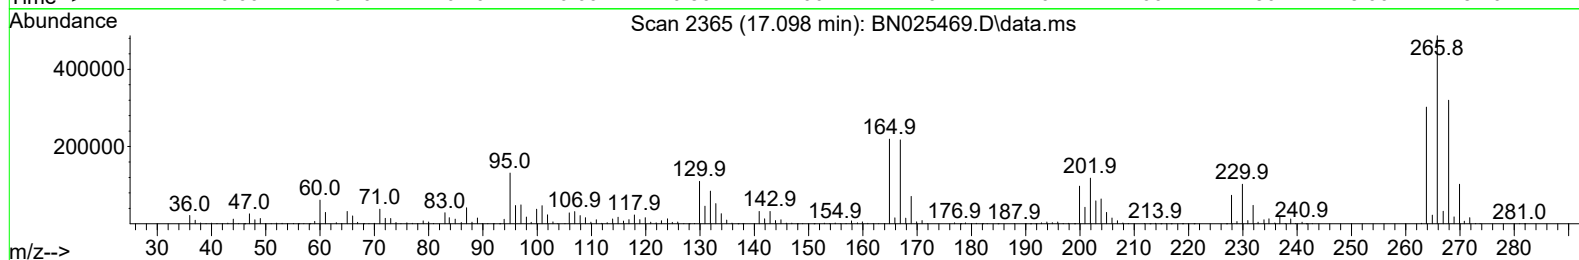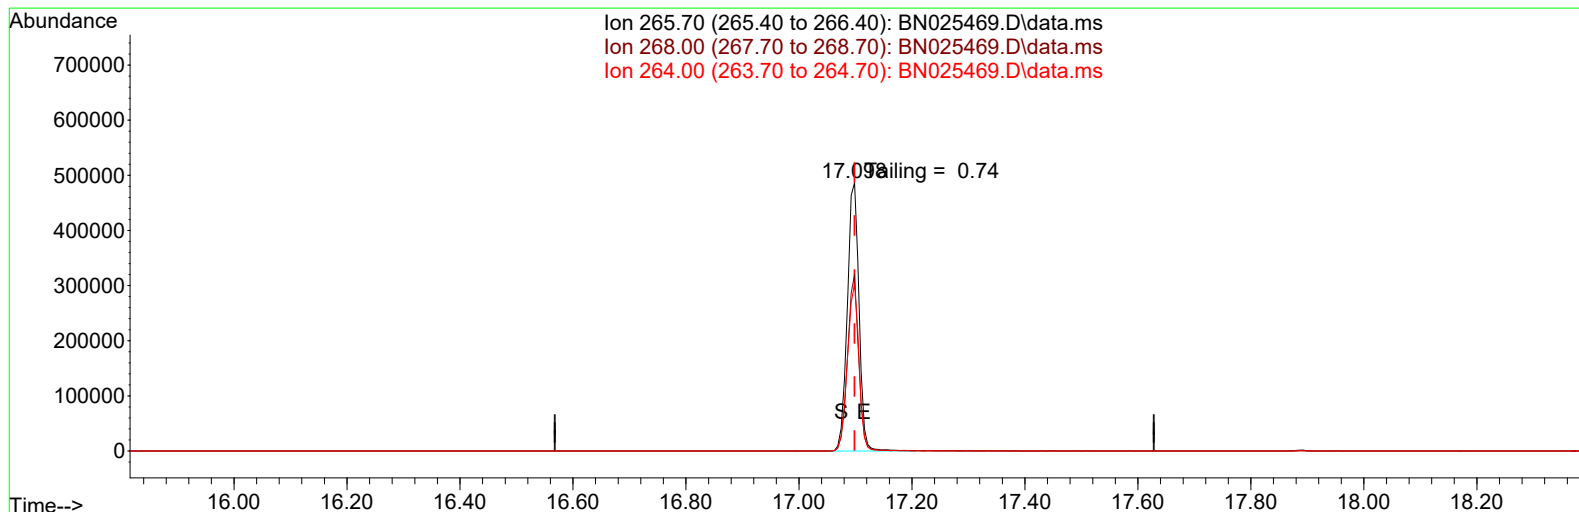

TIC: BN025469.D\data.ms

(70) Pentachlorophenol (C)

17.098min (0.000) 21655.13 ng




response 701189

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.74
264.00	61.60	62.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051823\
 Data File : BN025469.D
 Acq On : 18 May 2023 11:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 19 05:57:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 19 05:57:12 2023
 Response via : Initial Calibration

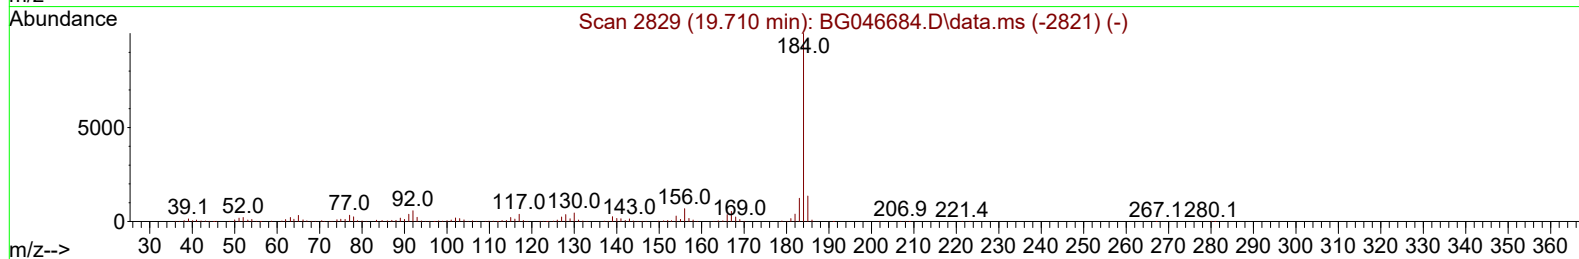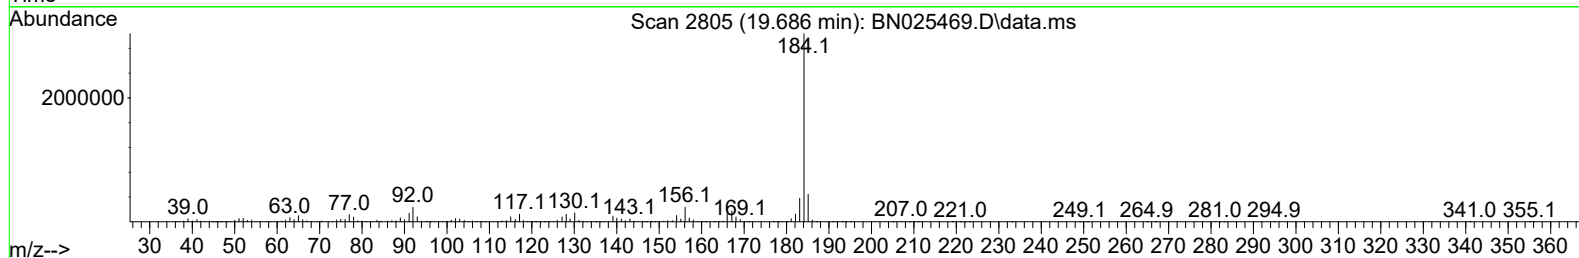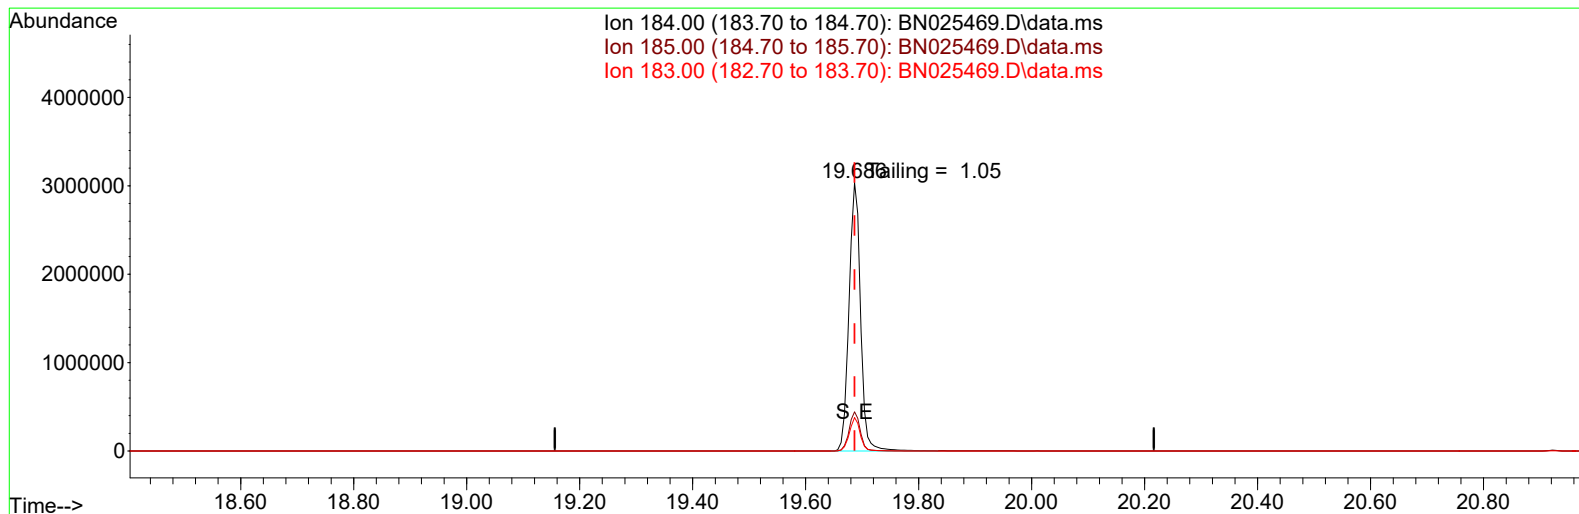

TIC: BN025469.D\data.ms

(77) Benzidine

19.686min (0.000) 2595362.65 ng

response 4320163

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.62
183.00	13.20	12.51
0.00	0.00	0.00