
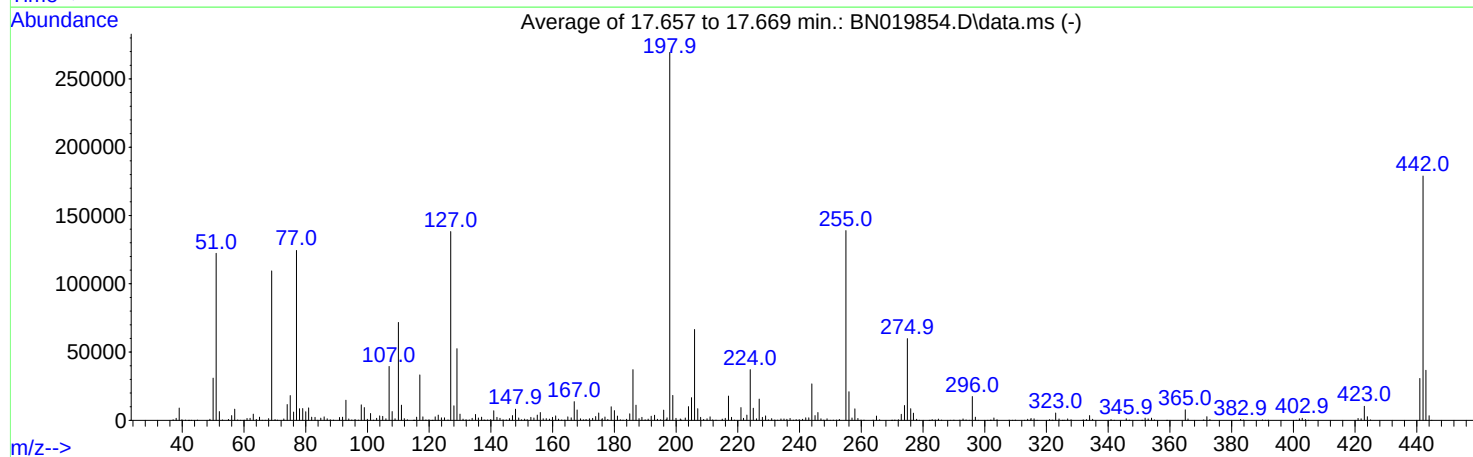


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051922\
 Data File : BN019854.D
 Acq On : 19 May 2022 14:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 18 07:42:52 2022

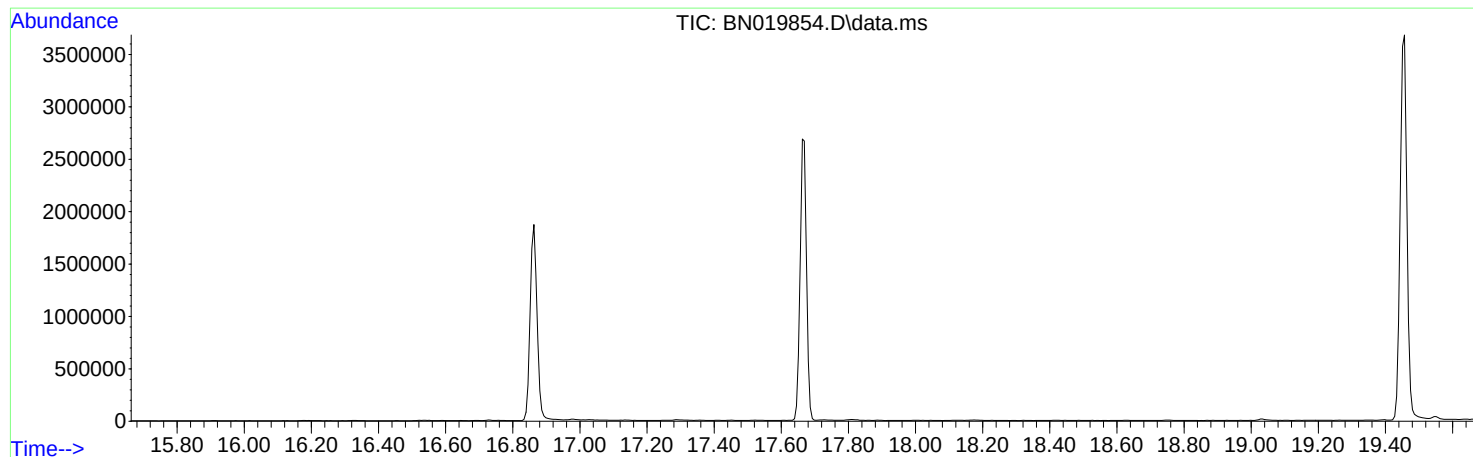




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	122286	PASS
68	69	0.00	2	1.2	1263	PASS
69	198	0.00	100	40.6	109411	PASS
70	69	0.00	2	0.6	602	PASS
127	198	10	80	51.3	138245	PASS
197	198	0.00	2	0.7	1859	PASS
198	198	100	100	100.0	269355	PASS
199	198	5	9	6.8	18241	PASS
275	198	10	60	22.2	59840	PASS
365	198	1	100	2.9	7692	PASS
441	198	0.01	100	11.4	30712	PASS
442	442	50	100	100.0	178915	PASS
443	442	15	24	20.5	36707	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051922\
 Data File : BN019854.D
 Acq On : 19 May 2022 14:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 20 07:19:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

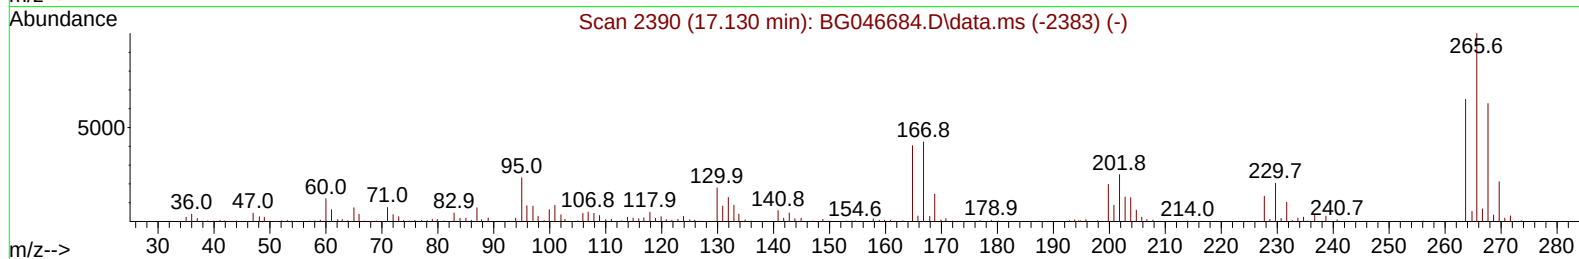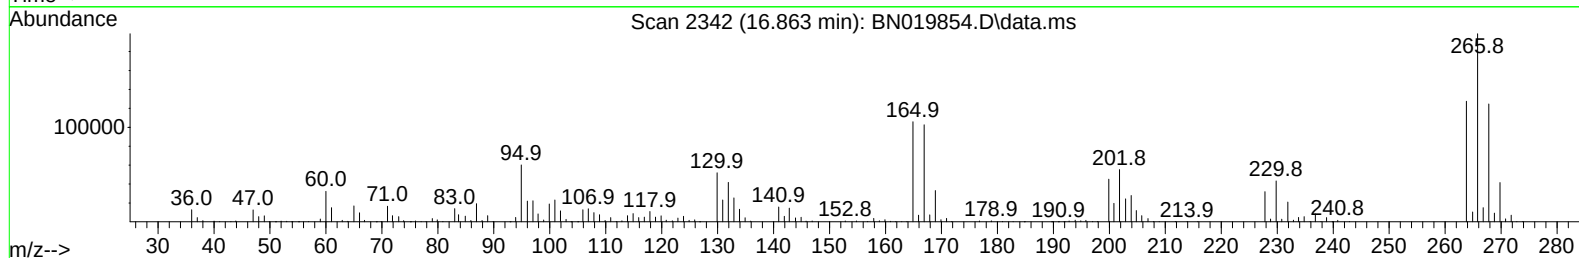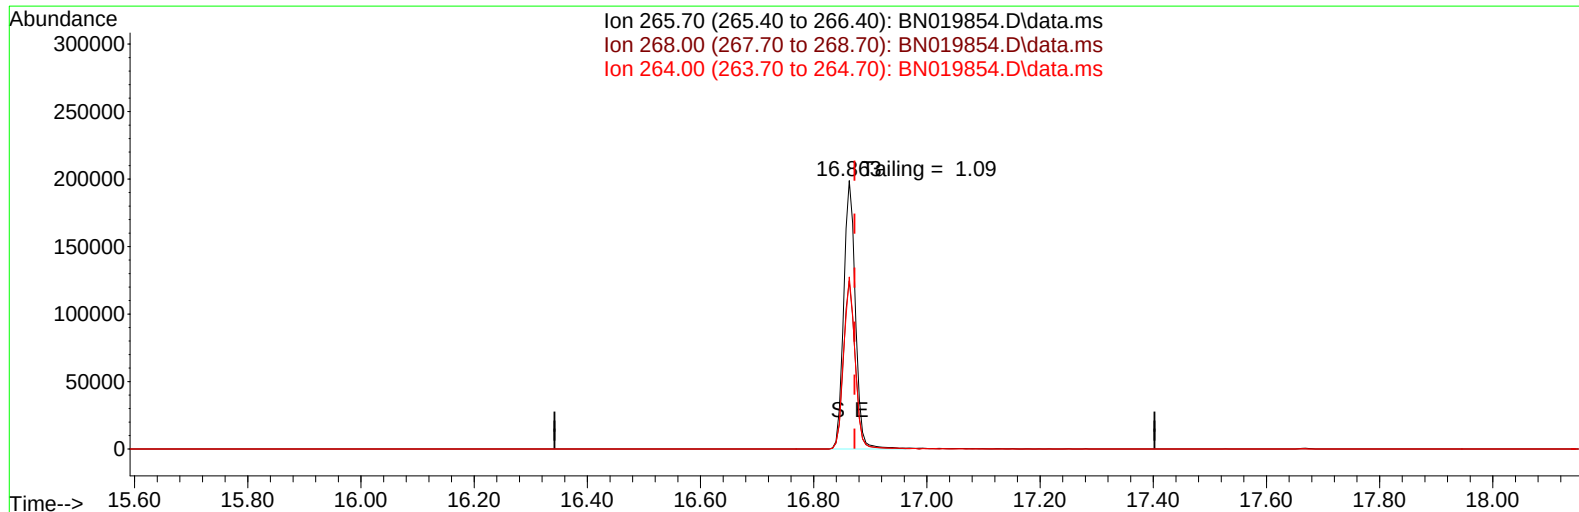

TIC: BN019854.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.009) 20036.60 ng




response 286967

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.64
264.00	61.60	64.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051922\
Data File : BN019854.D
Acq On : 19 May 2022 14:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 20 07:19:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

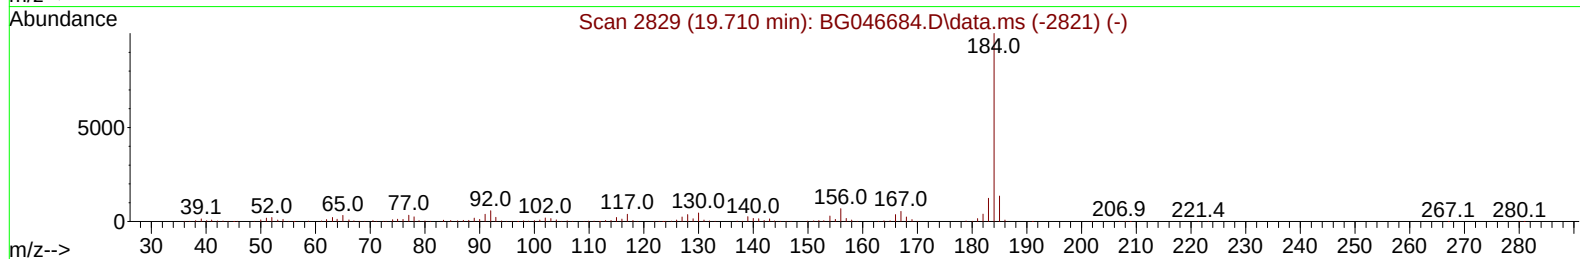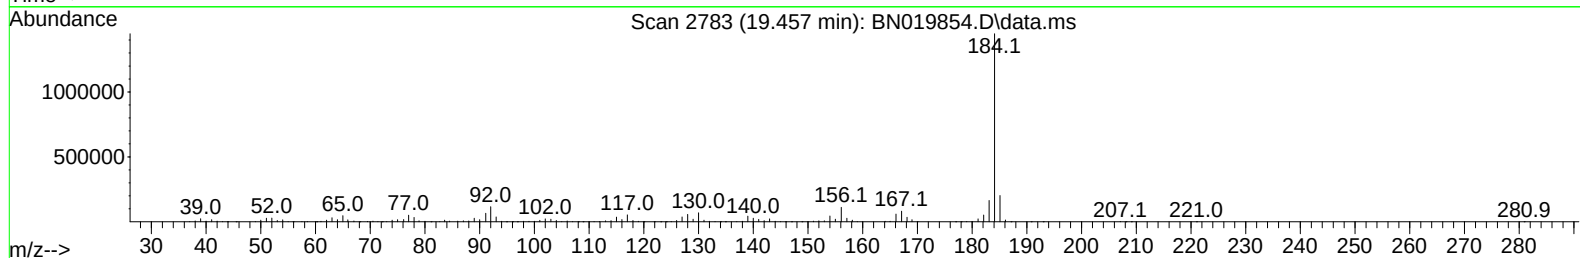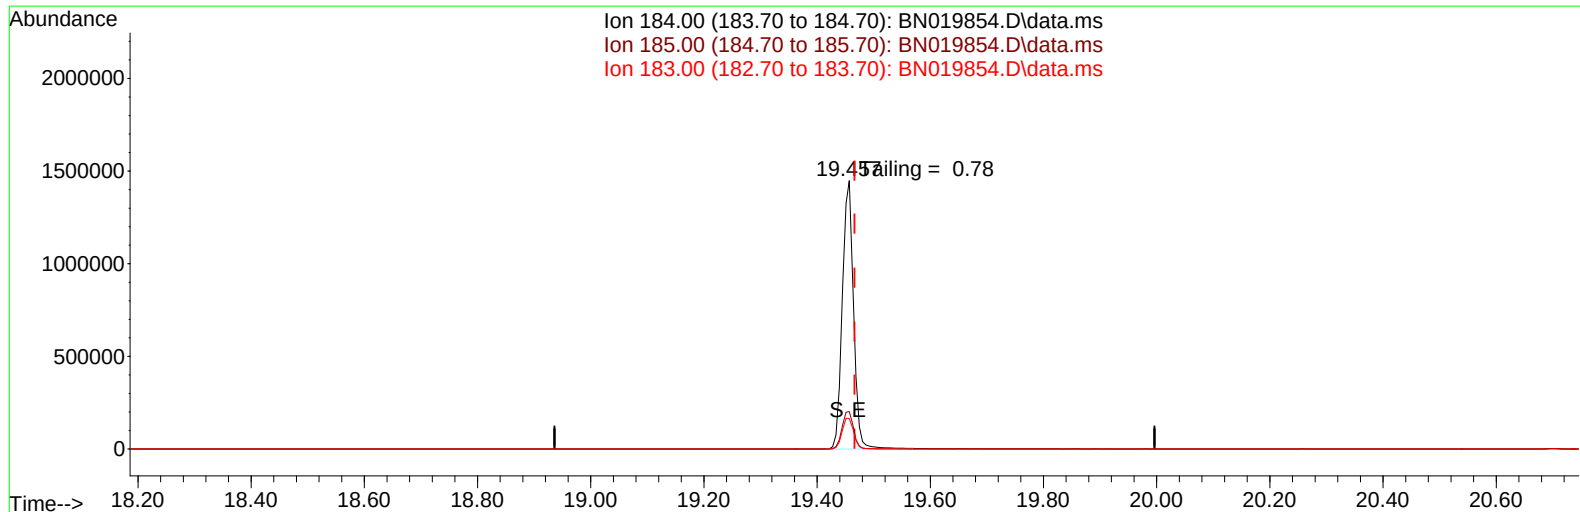

TIC: BN019854.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 2010805

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	11.36
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/19/2022	BNA_N	<u>BN019854.D</u>
Compound Name	Response	Retention Time
DDT	829646	20.704
DDD	112534	20.257
DDE	948	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
113482	943128	12.03

Instrument :
BNA_N
ClientSampleId :
DFTPP