
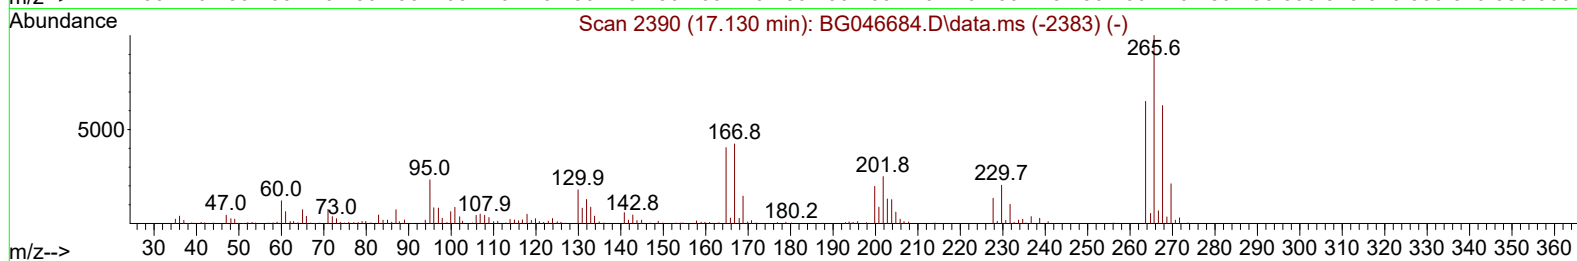
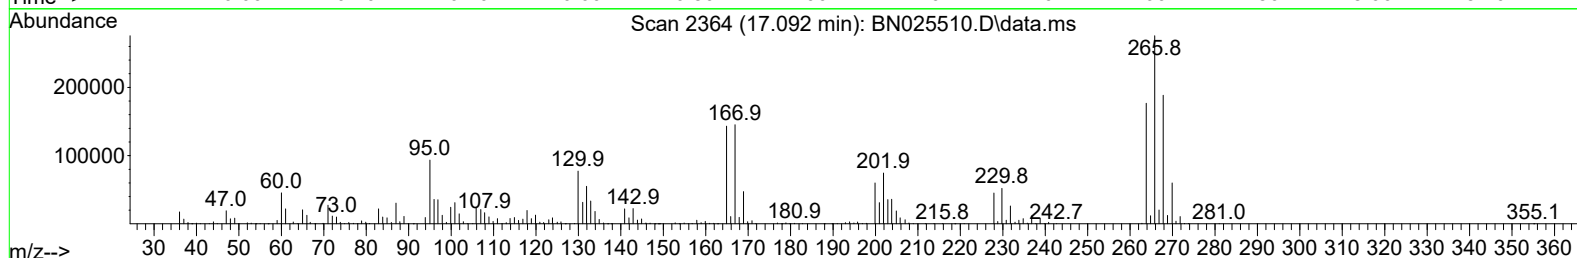


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051923\
Data File : BN025510.D
Acq On : 20 May 2023 05:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 03:37:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 22 03:37:34 2023
Response via : Initial Calibration

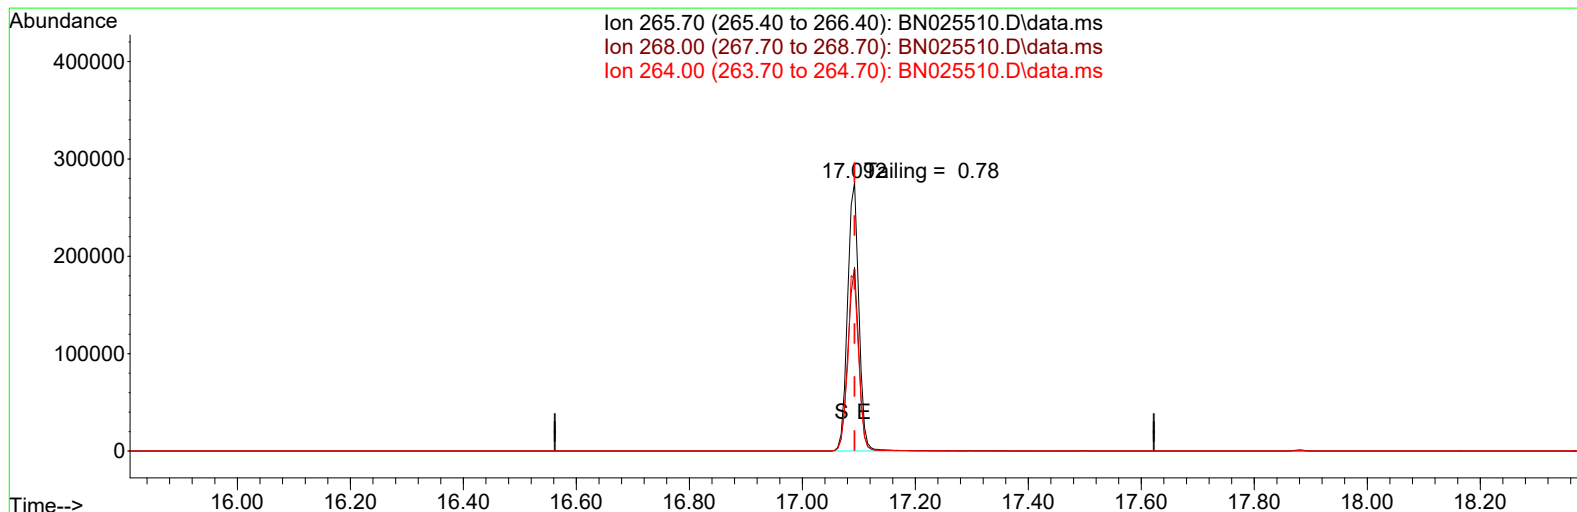

TIC: BN025510.D\data.ms

(70) Pentachlorophenol (C)




17.092min (0.000) 16828.88 ng

response 383660

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.33
264.00	61.60	64.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051923\
Data File : BN025510.D
Acq On : 20 May 2023 05:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 03:37:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 22 03:37:34 2023
Response via : Initial Calibration

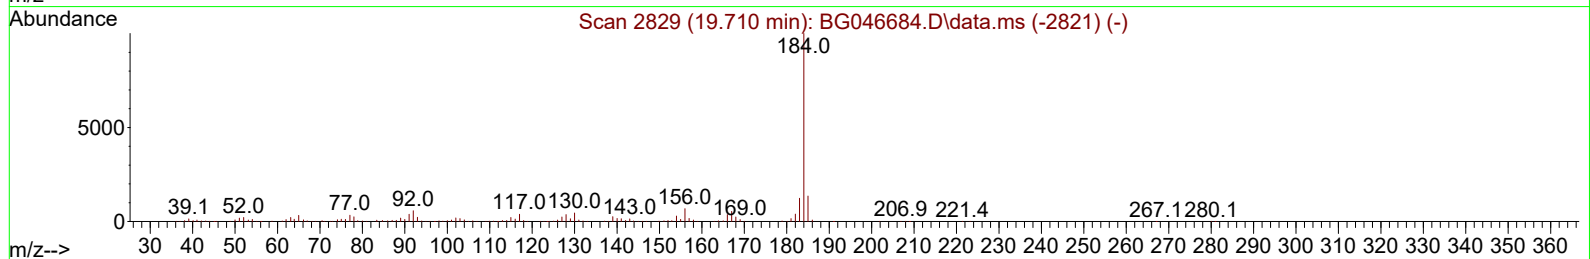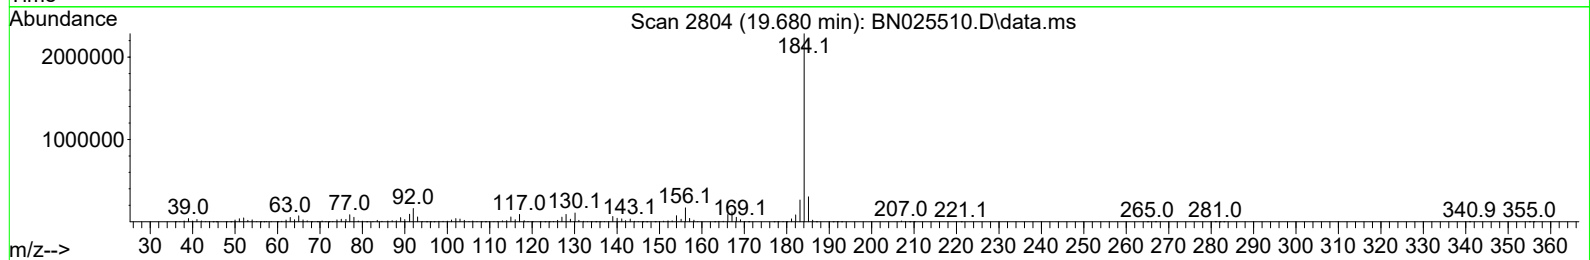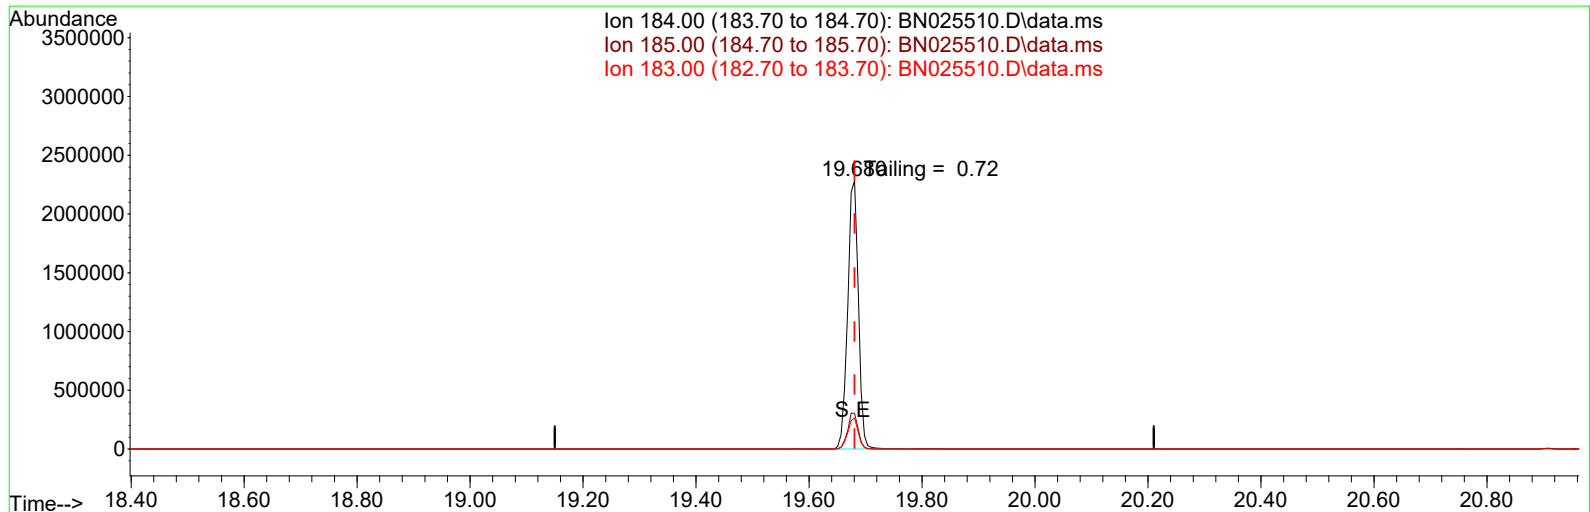

TIC: BN025510.D\data.ms

(77) Benzidine

19.680min (0.000) 0.00 ng

response 3010808

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.31
183.00	13.20	11.57
0.00	0.00	0.00