
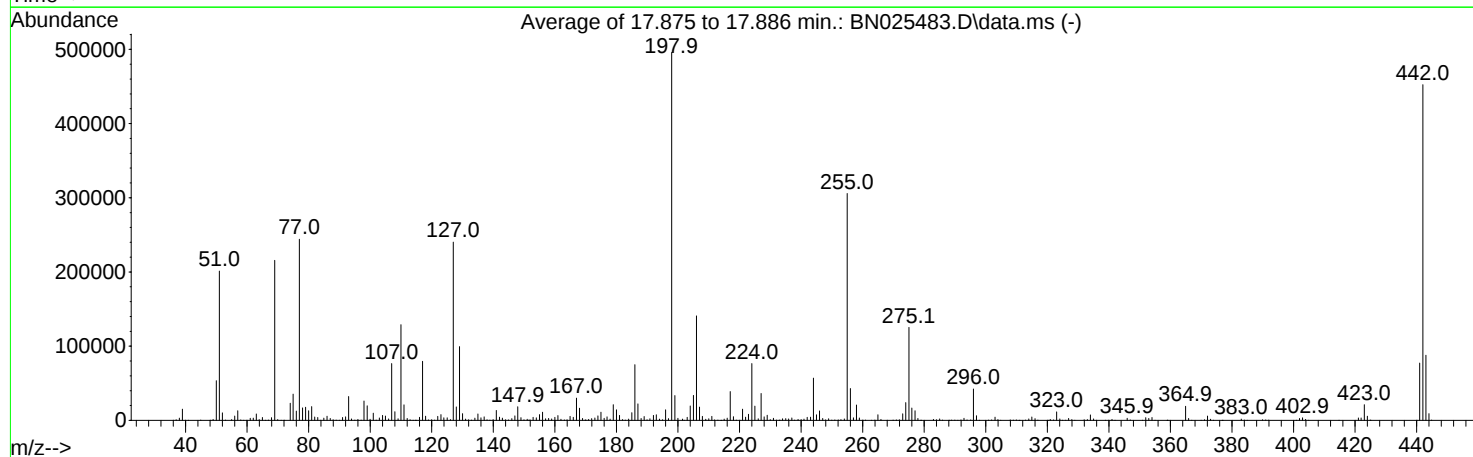


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051923\
 Data File : BN025483.D
 Acq On : 19 May 2023 09:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 22 01:54:38 2023

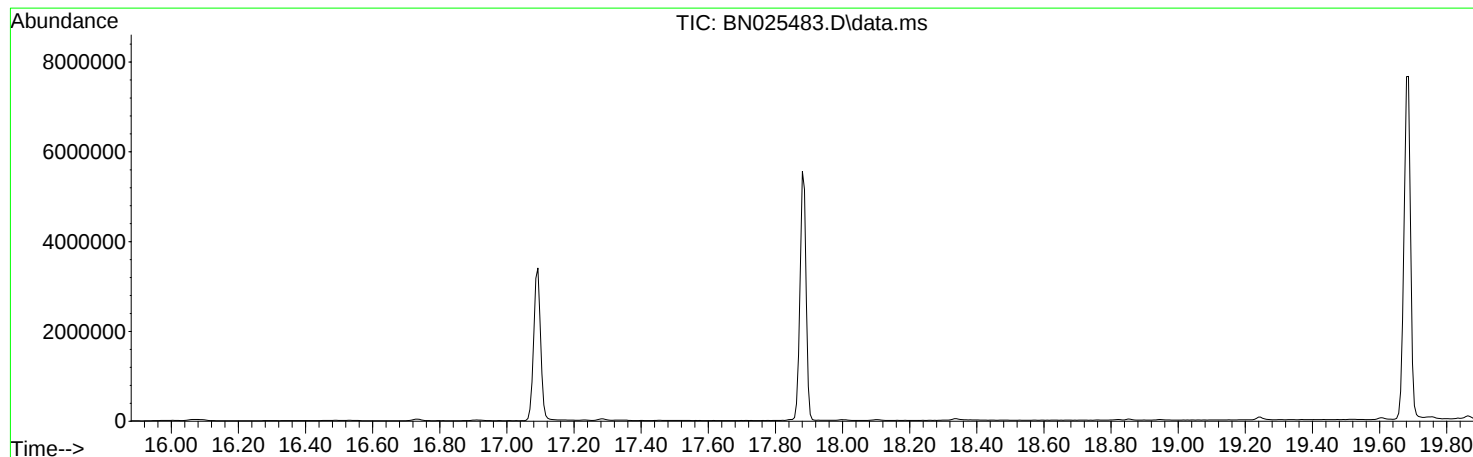

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	201237	PASS
68	69	0.00	2	1.8	3791	PASS
69	198	0.00	100	43.5	215775	PASS
70	69	0.00	2	0.5	1123	PASS
127	198	10	80	48.5	240341	PASS
197	198	0.00	2	0.5	2365	PASS
198	198	100	100	100.0	495787	PASS
199	198	5	9	6.7	33419	PASS
275	198	10	60	25.3	125256	PASS
365	198	1	100	3.8	18922	PASS
441	198	0.01	100	15.6	77128	PASS
442	442	50	100	100.0	452352	PASS
443	442	15	24	19.4	87872	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/19/2023	BNA_N	<u>BN025483.D</u>
Compound Name	Response	Retention Time
DDT	1886201	20.916
DDD	17013	20.527
DDE	152	19.969
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17165	1903366	0.90

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051923\
 Data File : BN025483.D
 Acq On : 19 May 2023 09:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 20 02:43:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 20 02:43:25 2023
 Response via : Initial Calibration

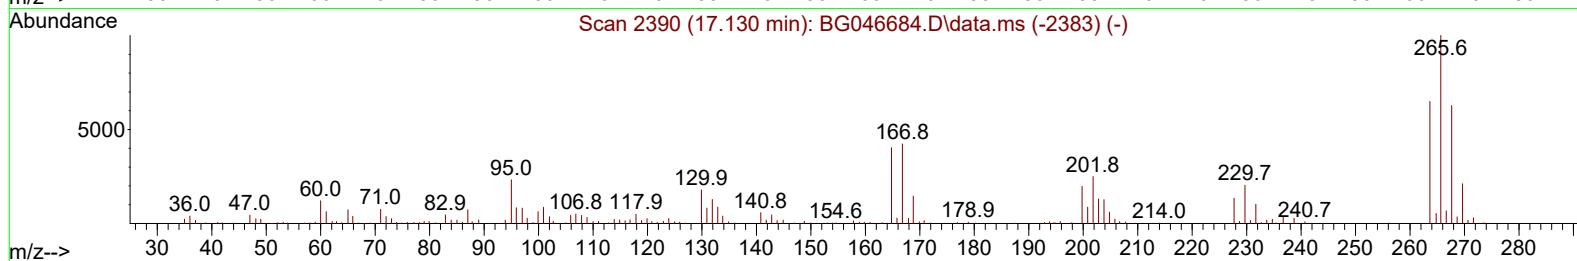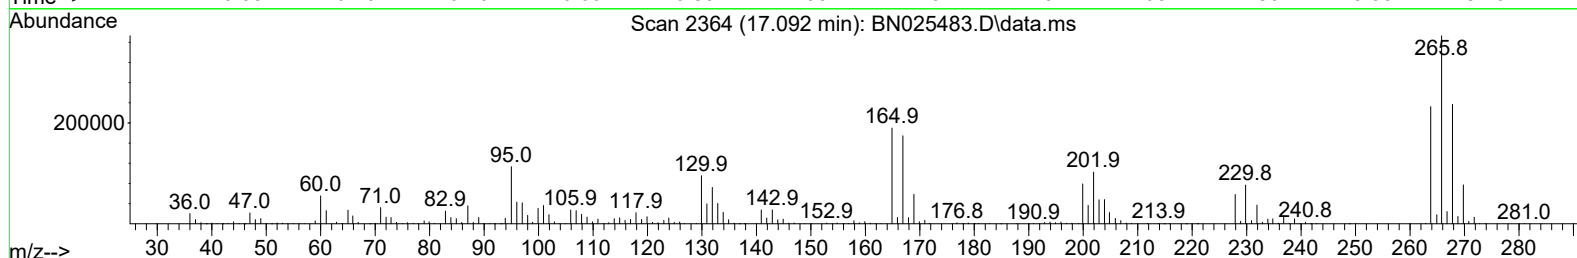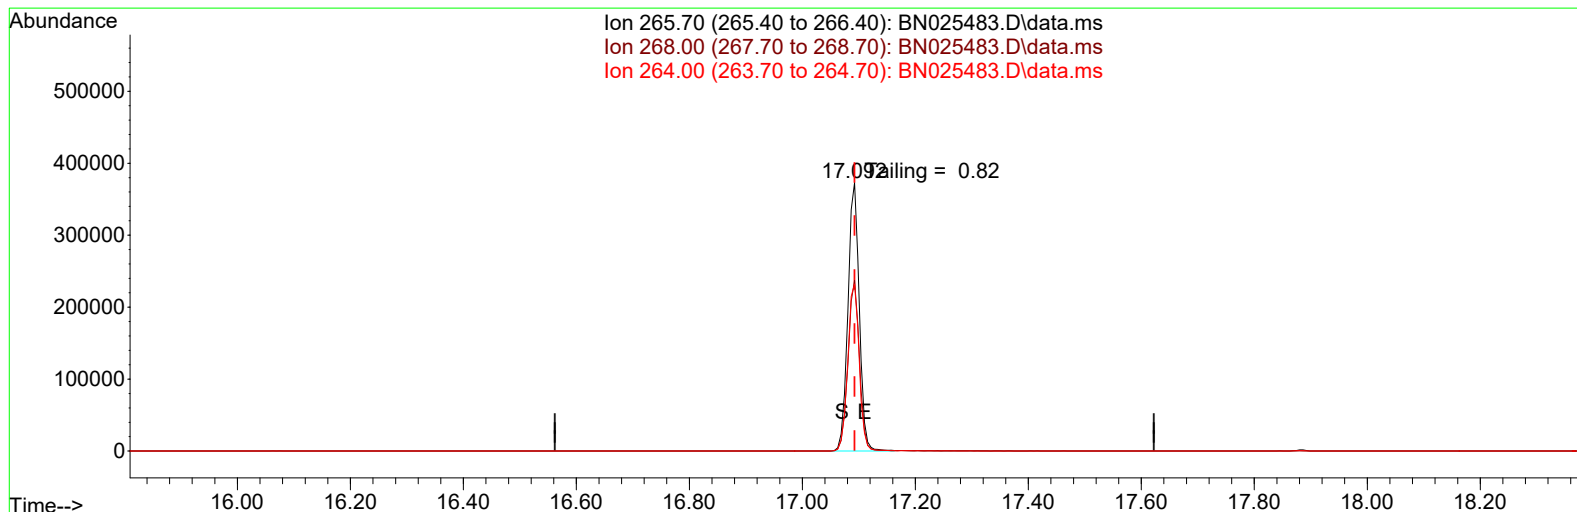

TIC: BN025483.D\data.ms

(70) Pentachlorophenol (C)

17.092min (0.000) 17958.94 ng




response 520763

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.49
264.00	61.60	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051923\
Data File : BN025483.D
Acq On : 19 May 2023 09:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 20 02:43:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 02:43:25 2023
Response via : Initial Calibration

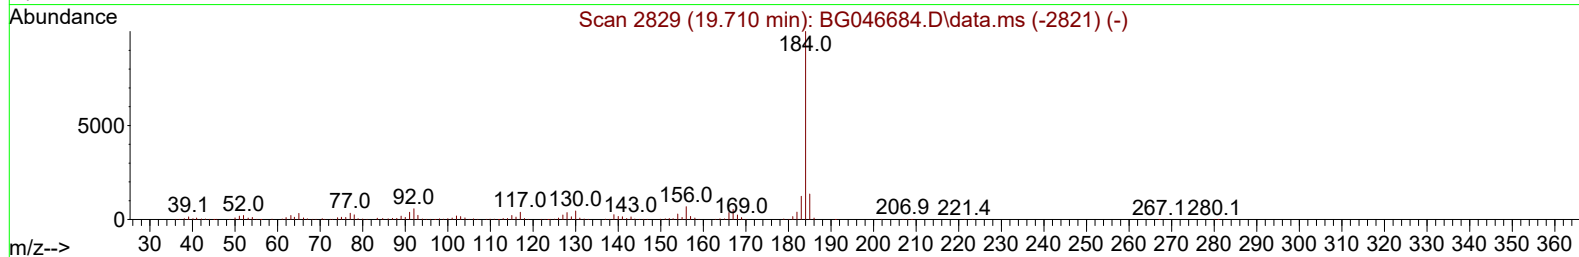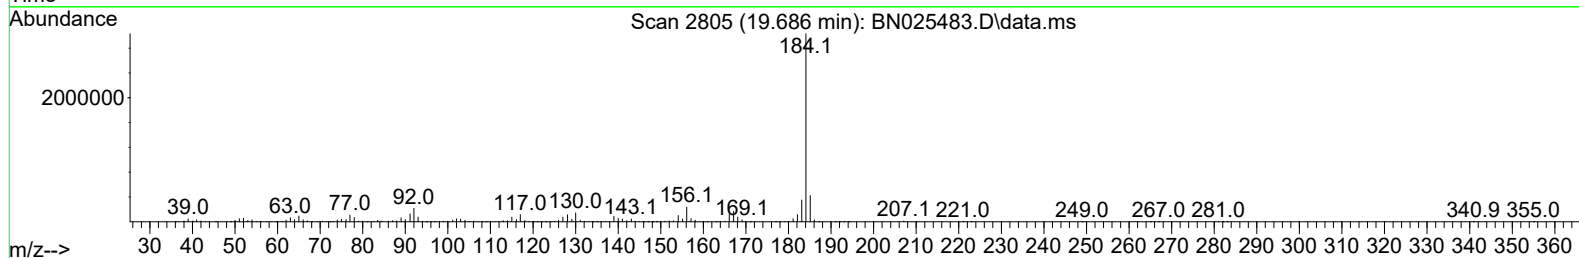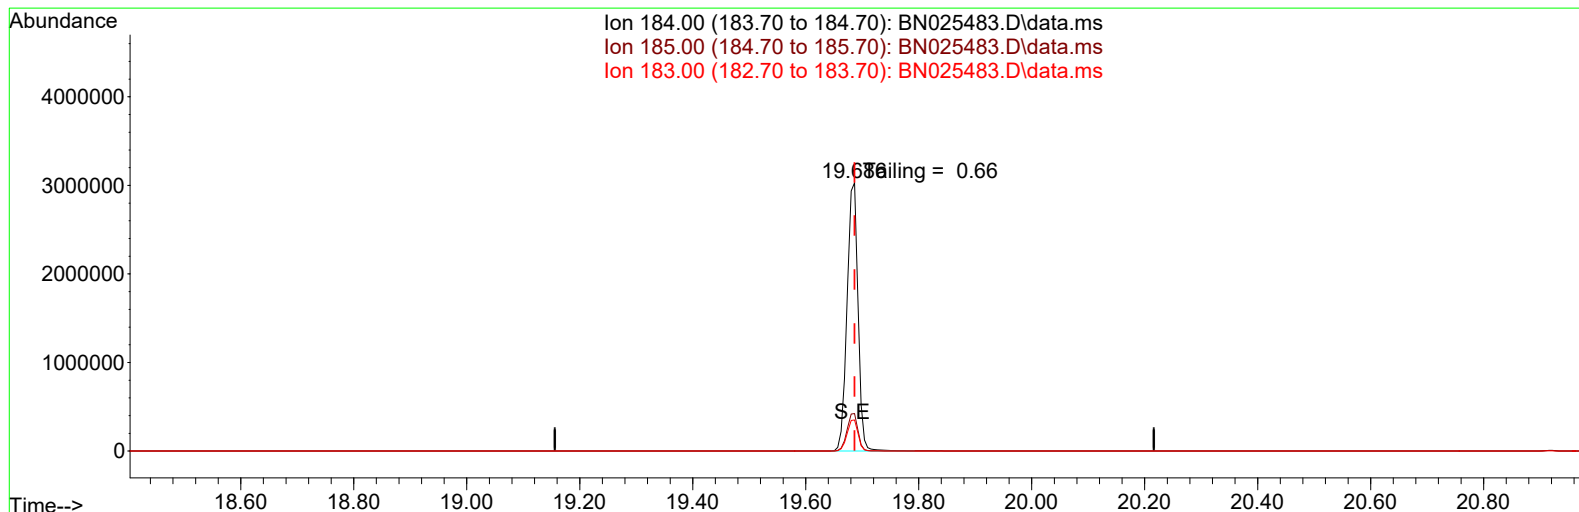

TIC: BN025483.D\data.ms

(77) Benzidine

19.686min (0.000) 2371529.74 ng

response 4093784

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	11.57
0.00	0.00	0.00