
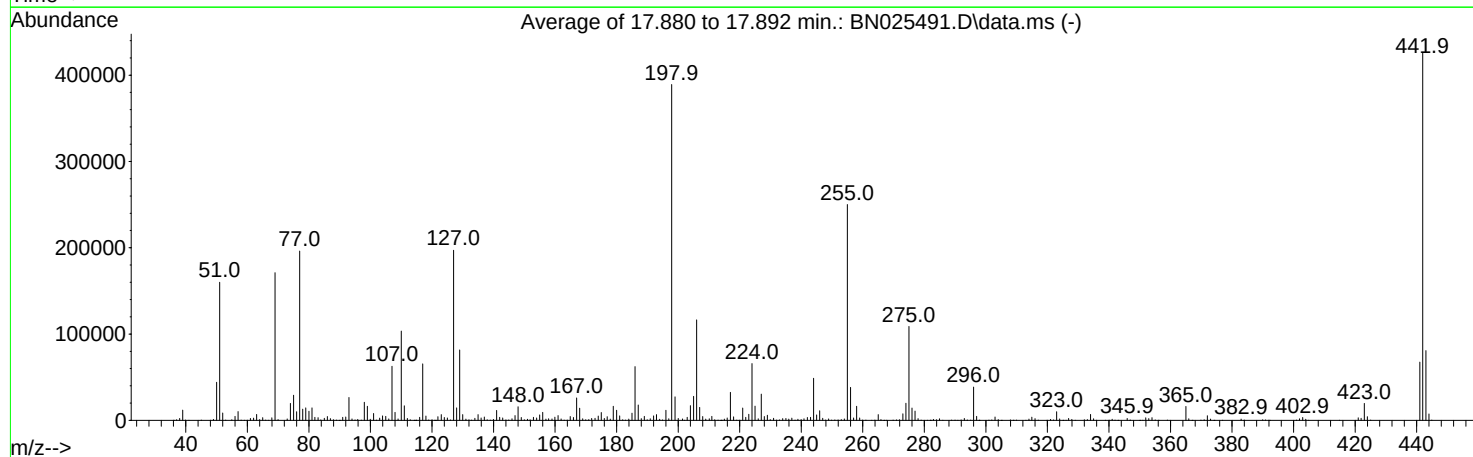


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051923\
 Data File : BN025491.D
 Acq On : 19 May 2023 17:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 22 01:54:38 2023

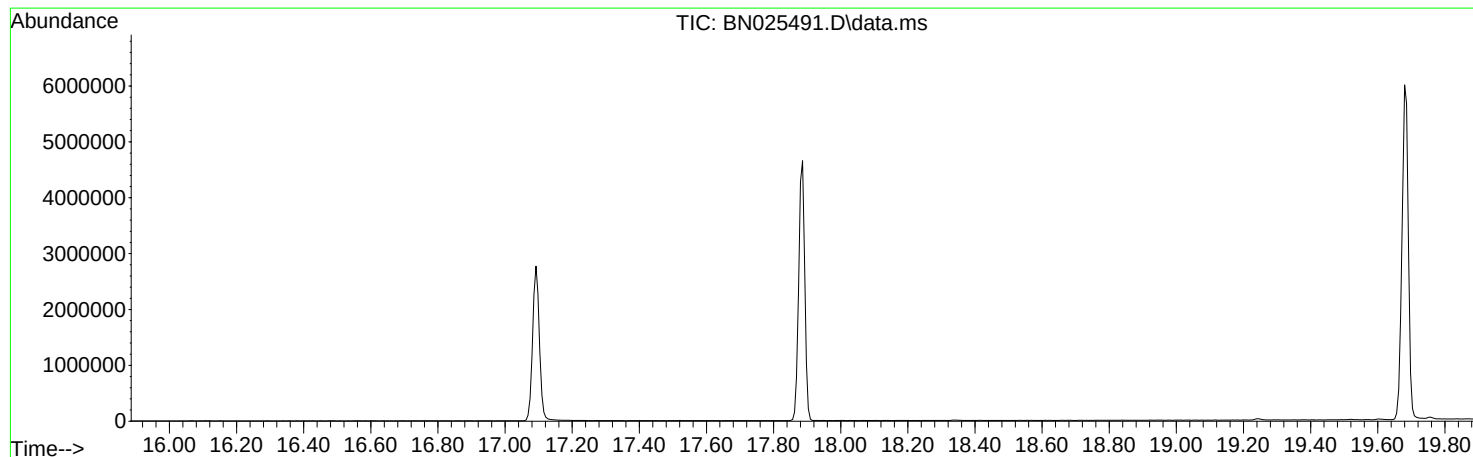

AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	160061	PASS
68	69	0.00	2	1.7	2955	PASS
69	198	0.00	100	44.0	171077	PASS
70	69	0.00	2	0.6	987	PASS
127	198	10	80	50.6	197035	PASS
197	198	0.00	2	0.5	1829	PASS
198	198	100	100	100.0	389205	PASS
199	198	5	9	7.0	27211	PASS
275	198	10	60	28.0	108821	PASS
365	198	1	100	4.1	16123	PASS
441	198	0.01	100	17.3	67419	PASS
442	442	50	100	100.0	426261	PASS
443	442	15	24	18.9	80755	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/19/2023	BNA_N	<u>BN025491.D</u>
Compound Name	Response	Retention Time
DDT	1417822	20.915
DDD	13778	20.527
DDE	0	19.969
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13778	1431600	0.96

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051923\
Data File : BN025491.D
Acq On : 19 May 2023 17:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 20 02:45:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 02:43:25 2023
Response via : Initial Calibration

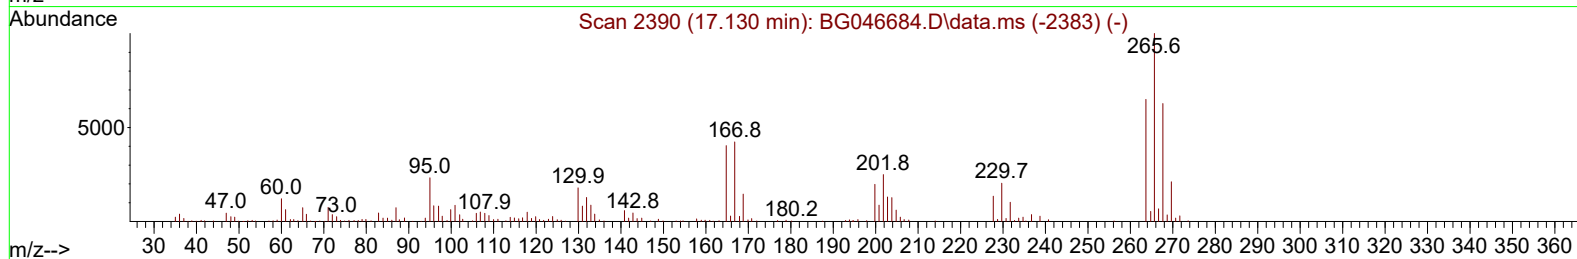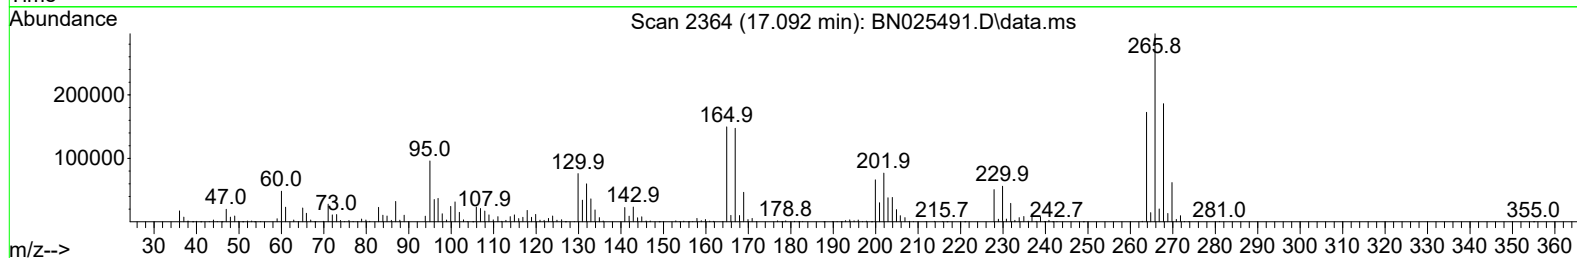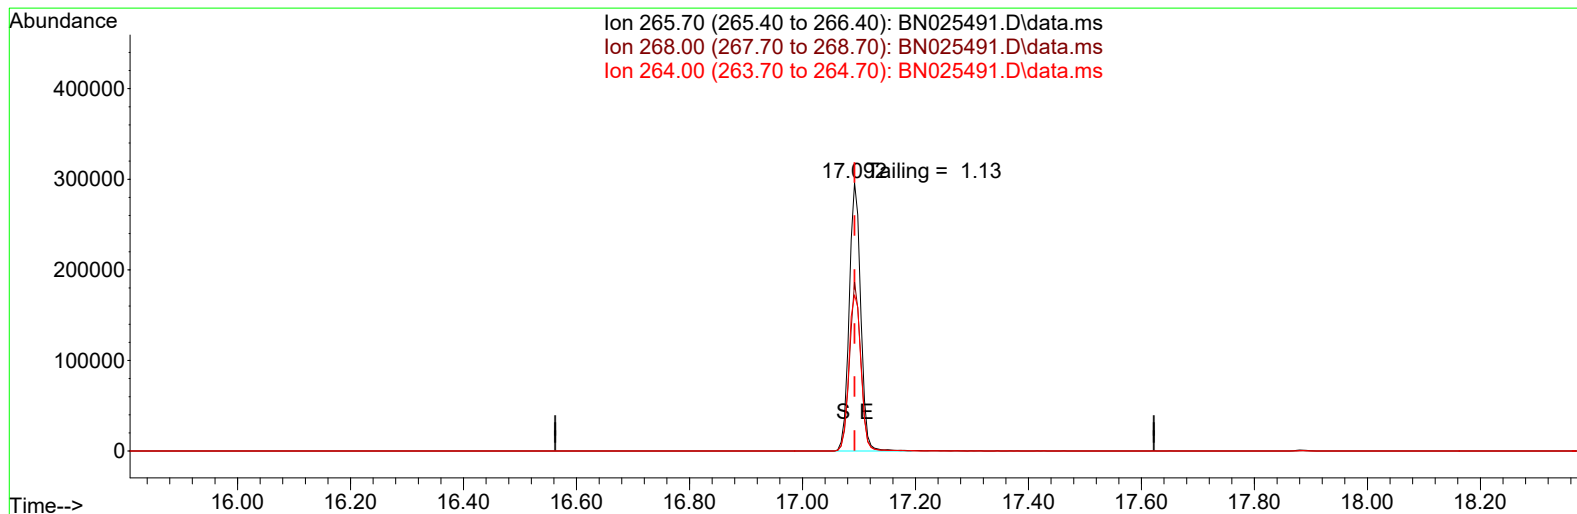

TIC: BN025491.D\data.ms

(70) Pentachlorophenol (C)

17.092min (-0.000) 17796.13 ng




response 419677

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.86
264.00	61.60	58.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051923\
Data File : BN025491.D
Acq On : 19 May 2023 17:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 20 02:45:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 02:43:25 2023
Response via : Initial Calibration

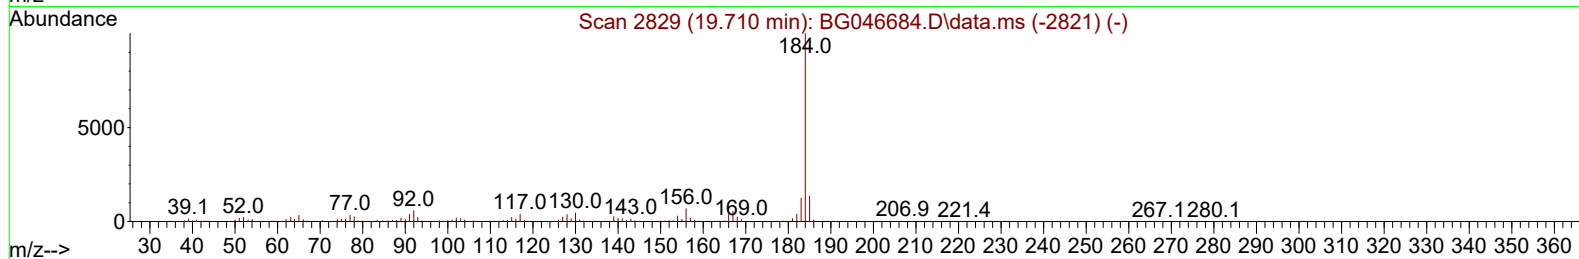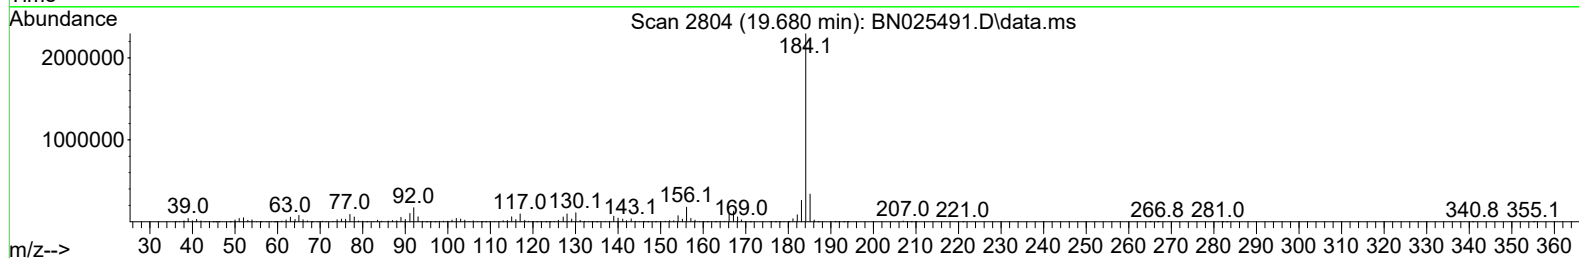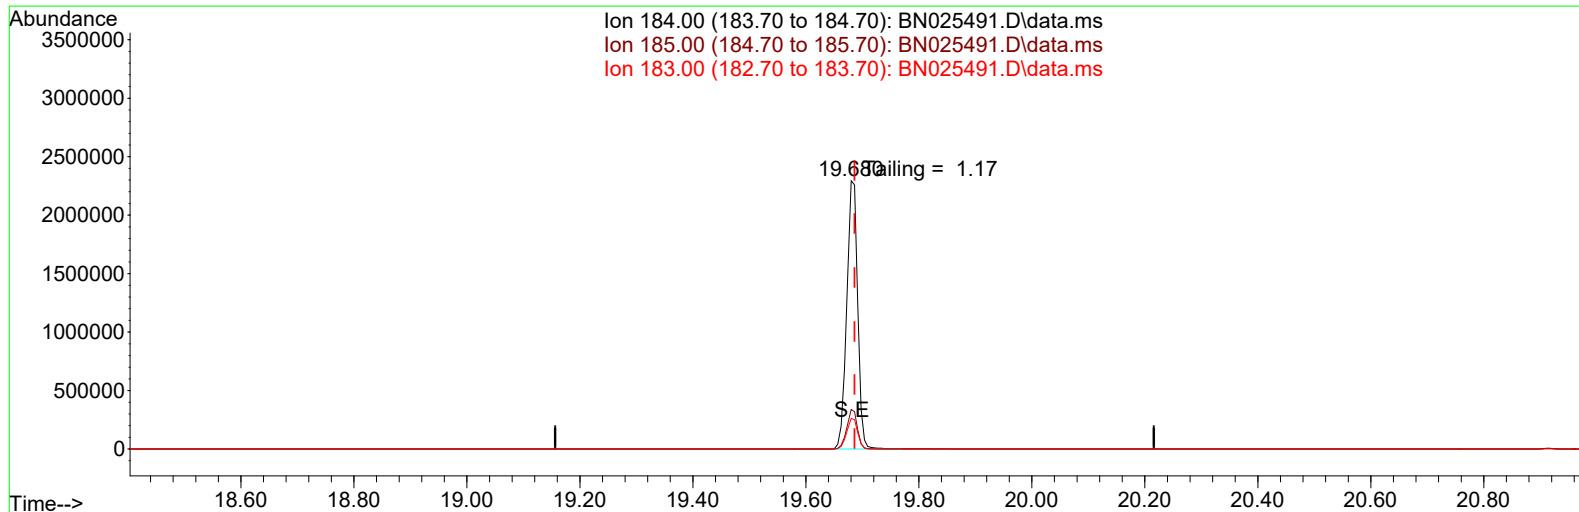

TIC: BN025491.D\data.ms

(77) Benzidine

19.680min (-0.006) 0.00 ng

response 3084782

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.73
183.00	13.20	11.42
0.00	0.00	0.00