
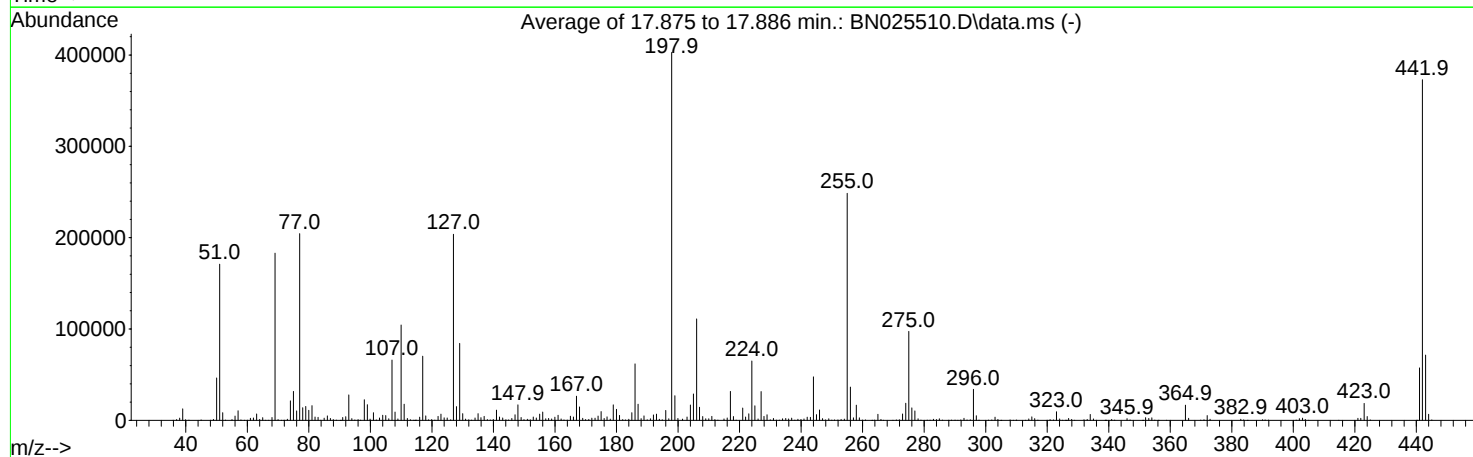


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051923\
 Data File : BN025510.D
 Acq On : 20 May 2023 05:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 22 01:54:38 2023

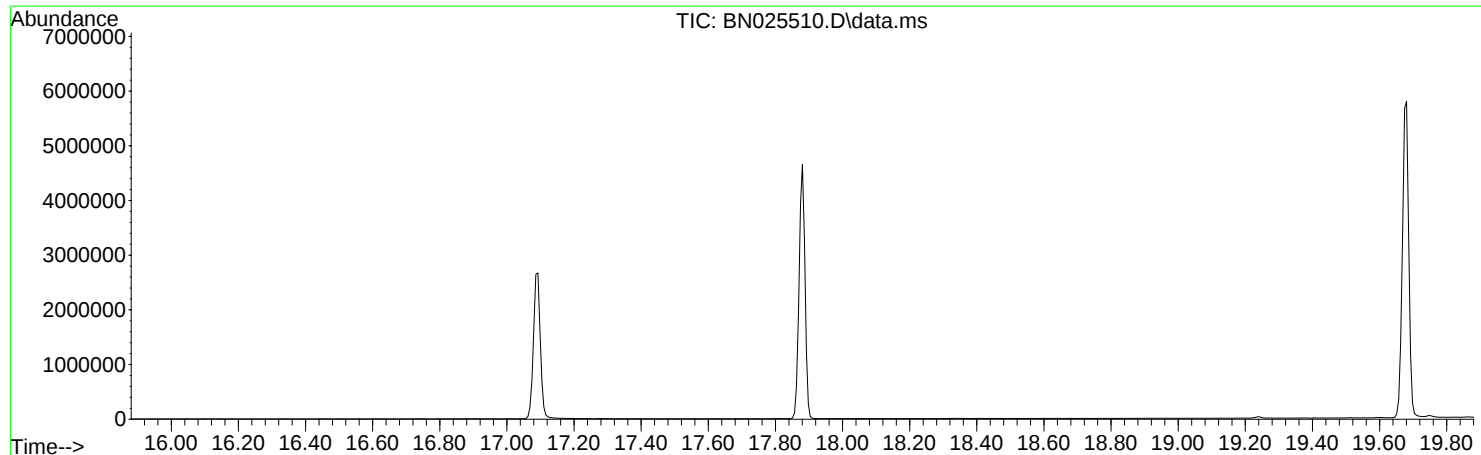

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	170904	PASS
68	69	0.00	2	1.7	3091	PASS
69	198	0.00	100	45.5	183104	PASS
70	69	0.00	2	0.5	918	PASS
127	198	10	80	50.6	203755	PASS
197	198	0.00	2	0.5	1840	PASS
198	198	100	100	100.0	402731	PASS
199	198	5	9	6.7	27043	PASS
275	198	10	60	24.2	97405	PASS
365	198	1	100	4.1	16709	PASS
441	198	0.01	100	14.3	57485	PASS
442	442	50	100	100.0	372885	PASS
443	442	15	24	19.2	71536	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/19/2023	BNA_N	BN025510.D
Compound Name	Response	Retention Time
DDT	1389329	20.91
DDD	14158	20.521
DDE	0	19.969
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14158	1403487	1.01

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051923\
 Data File : BN025510.D
 Acq On : 20 May 2023 05:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 22 03:37:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 22 03:37:34 2023
 Response via : Initial Calibration

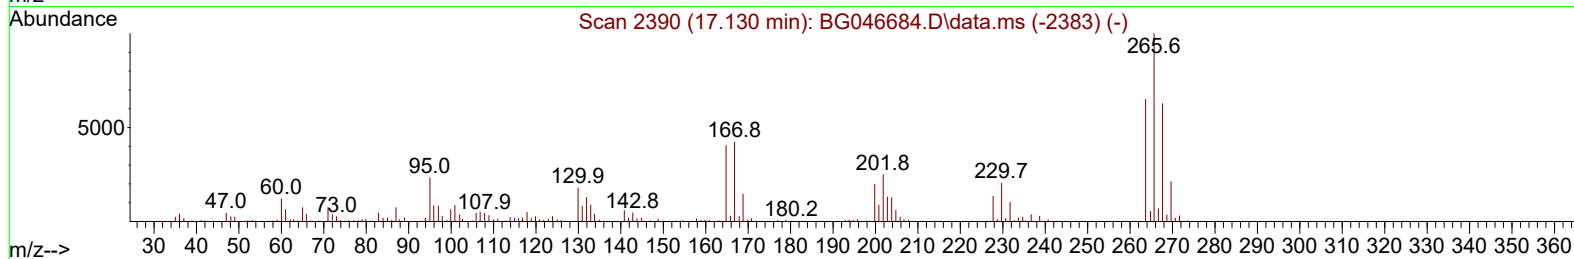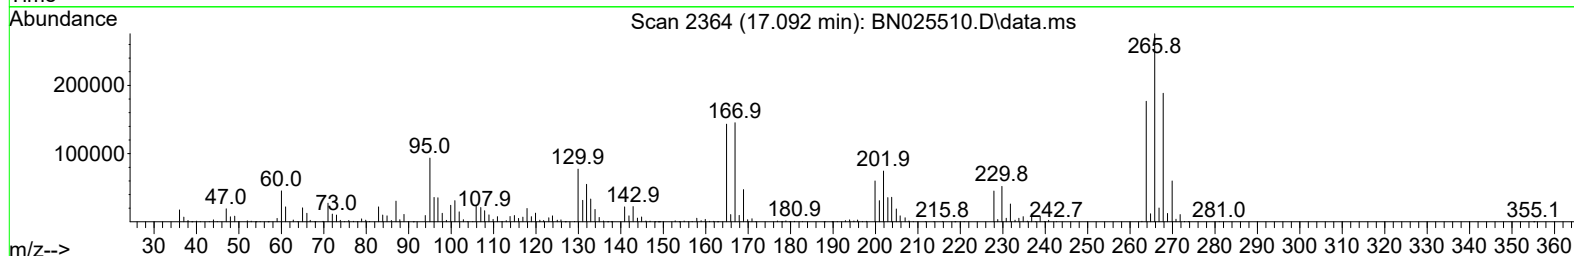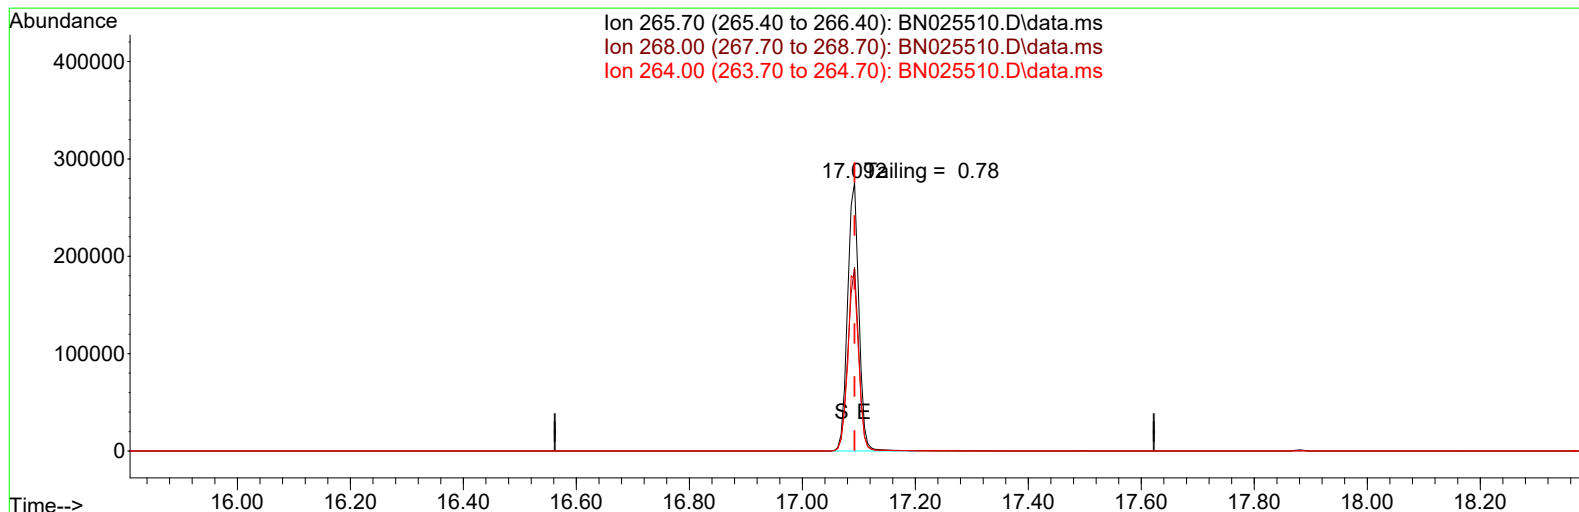

TIC: BN025510.D\data.ms

(70) Pentachlorophenol (C)

17.092min (0.000) 16828.88 ng




response 383660

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.33
264.00	61.60	64.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051923\
 Data File : BN025510.D
 Acq On : 20 May 2023 05:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 22 03:37:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 22 03:37:34 2023
 Response via : Initial Calibration

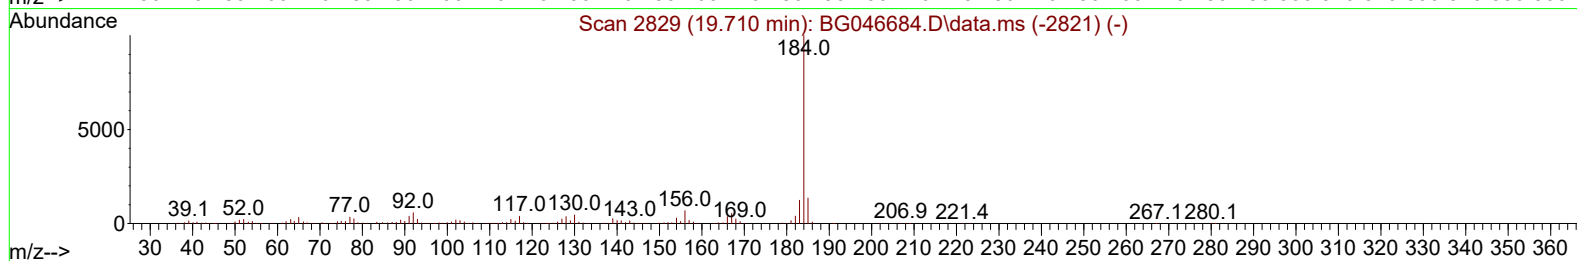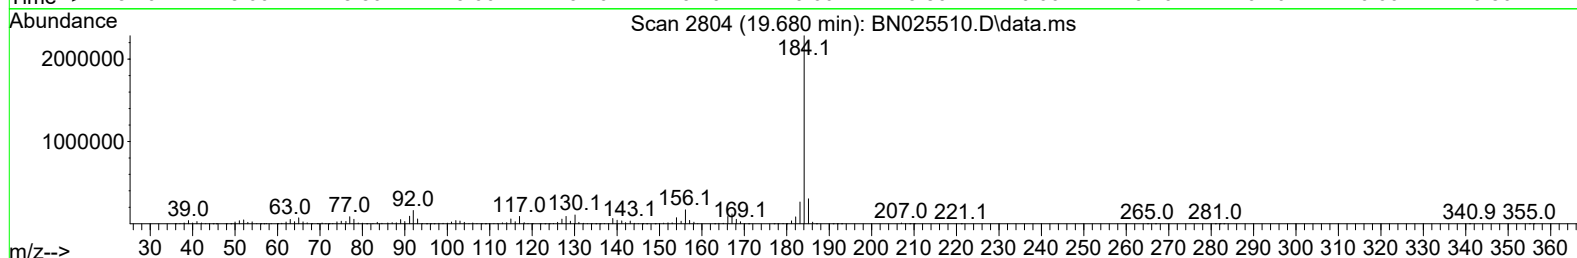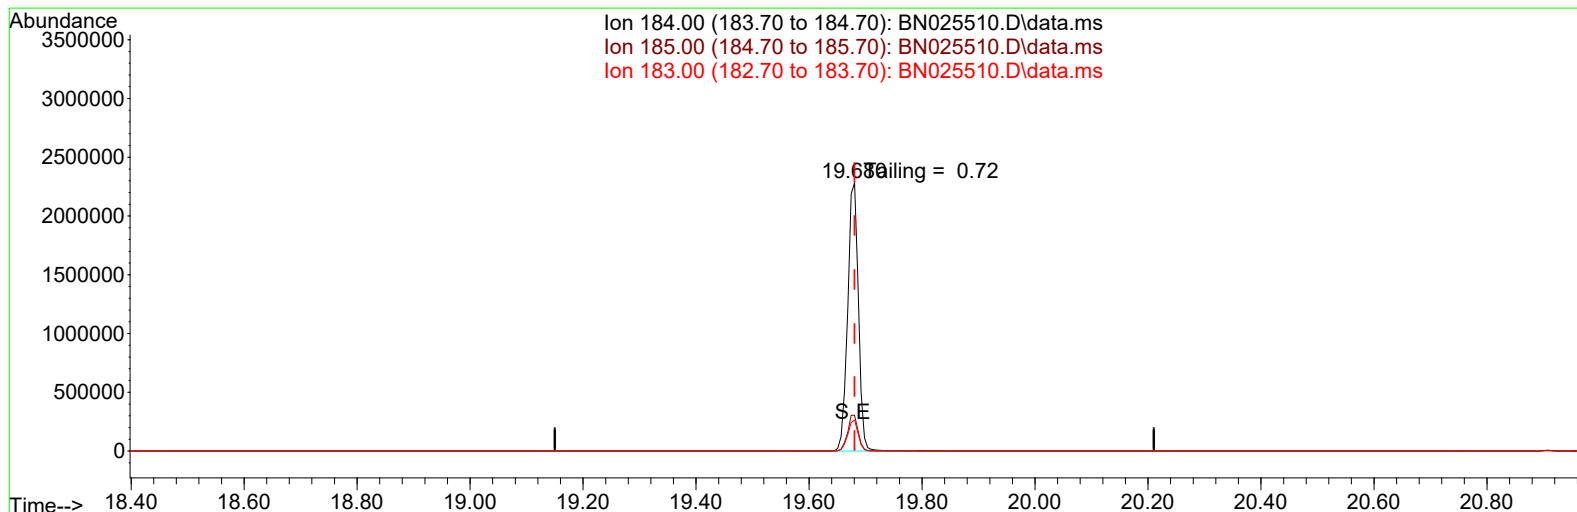

TIC: BN025510.D\data.ms

(77) Benzidine

19.680min (0.000) 0.00 ng

response 3010808

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.31
183.00	13.20	11.57
0.00	0.00	0.00