
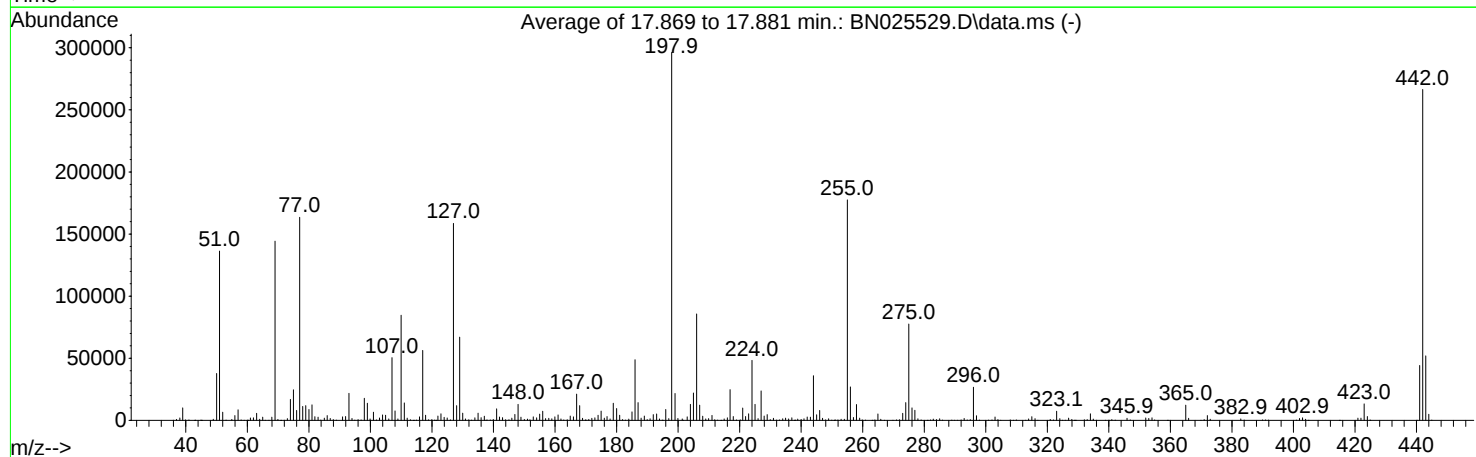


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051923\
 Data File : BN025529.D
 Acq On : 20 May 2023 18:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 22 01:54:38 2023

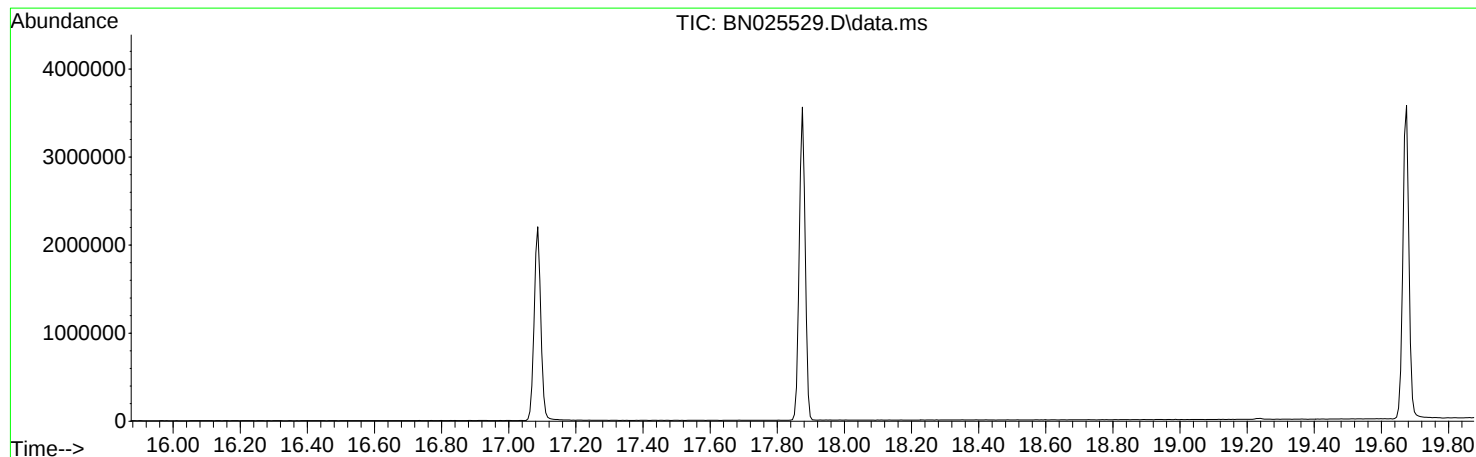

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	136298	PASS
68	69	0.00	2	1.8	2545	PASS
69	198	0.00	100	48.7	144248	PASS
70	69	0.00	2	0.5	781	PASS
127	198	10	80	53.6	158613	PASS
197	198	0.00	2	0.5	1417	PASS
198	198	100	100	100.0	296192	PASS
199	198	5	9	7.3	21627	PASS
275	198	10	60	26.2	77603	PASS
365	198	1	100	4.2	12316	PASS
441	198	0.01	100	14.9	44179	PASS
442	442	50	100	100.0	266432	PASS
443	442	15	24	19.5	51976	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/19/2023	BNA_N	<u>BN025529.D</u>
Compound Name	Response	Retention Time
DDT	882806	20.91
DDD	9174	20.522
DDE	0	19.969
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9174	891980	1.03

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051923\
 Data File : BN025529.D
 Acq On : 20 May 2023 18:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 22 03:39:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 22 03:37:34 2023
 Response via : Initial Calibration

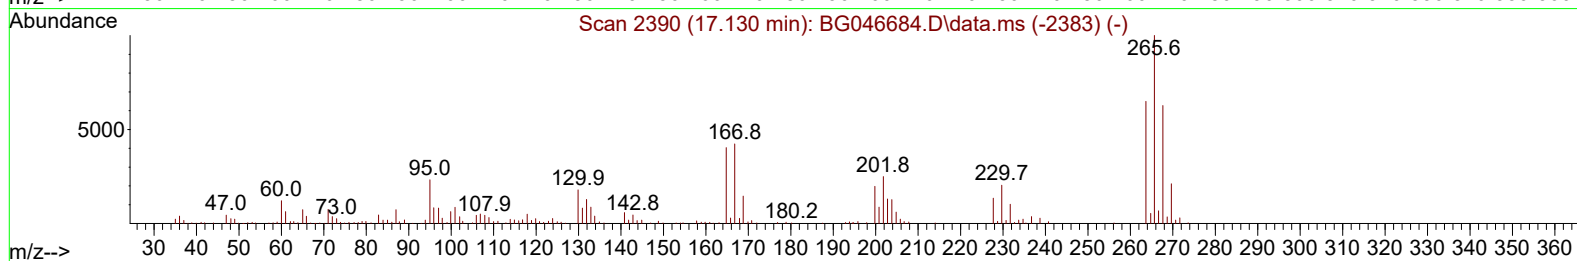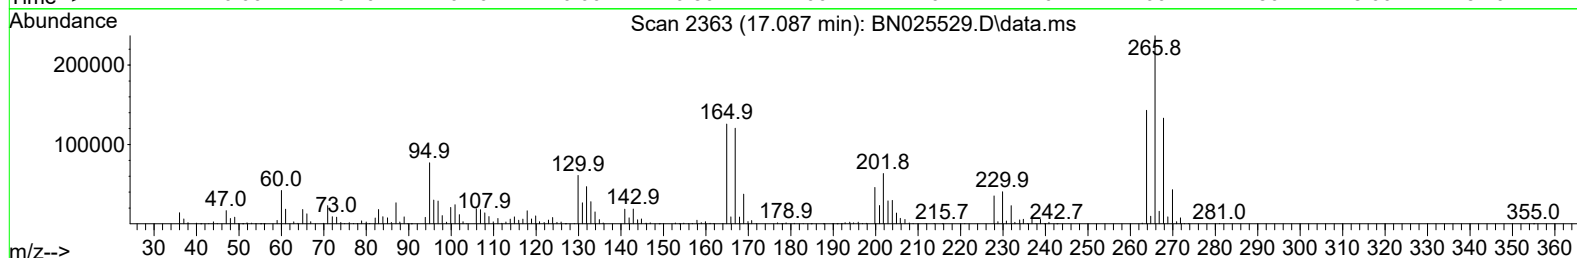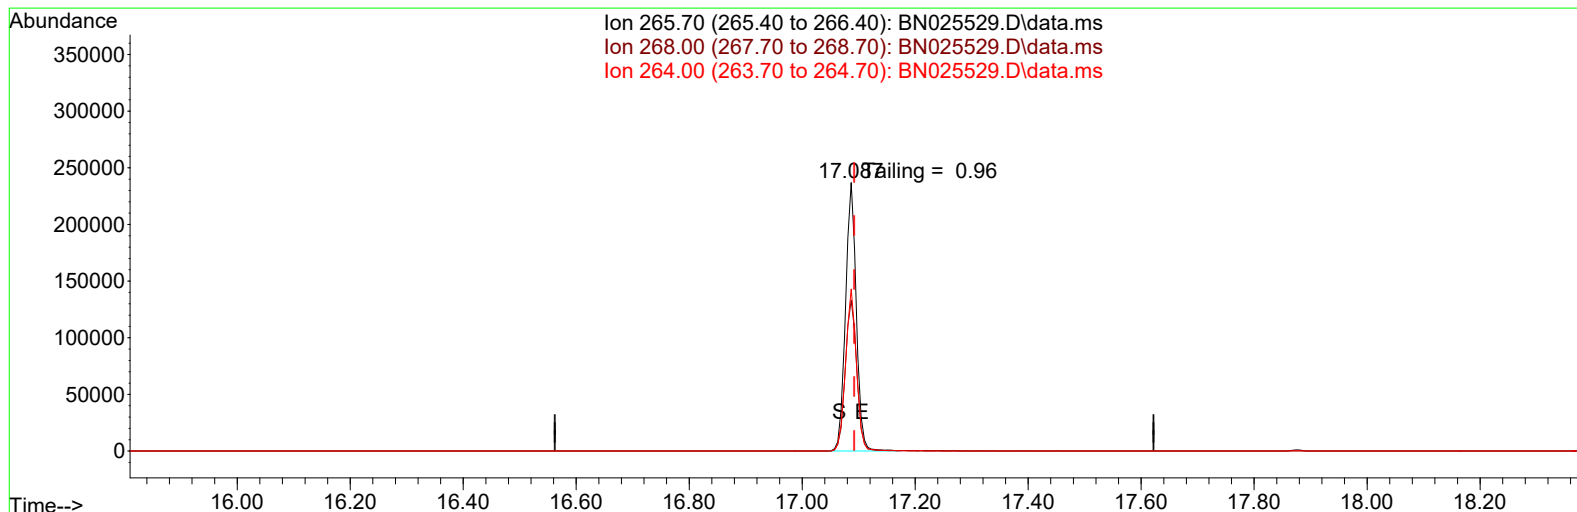

TIC: BN025529.D\data.ms

(70) Pentachlorophenol (C)

17.087min (-0.006) 16797.22 ng




response 312546

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	56.24
264.00	61.60	60.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051923\
Data File : BN025529.D
Acq On : 20 May 2023 18:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 22 03:39:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 22 03:37:34 2023
Response via : Initial Calibration

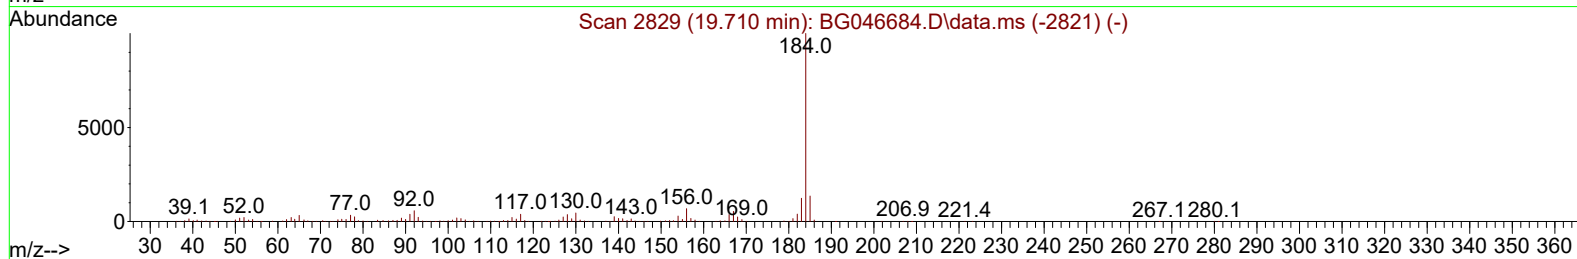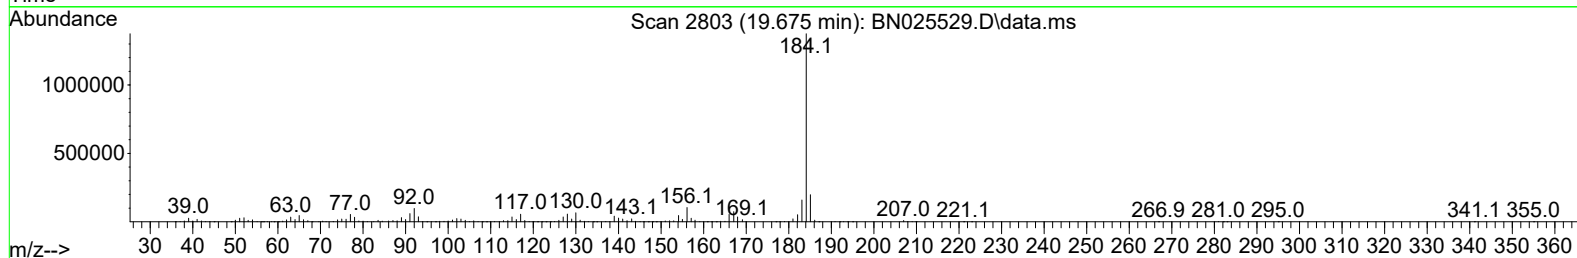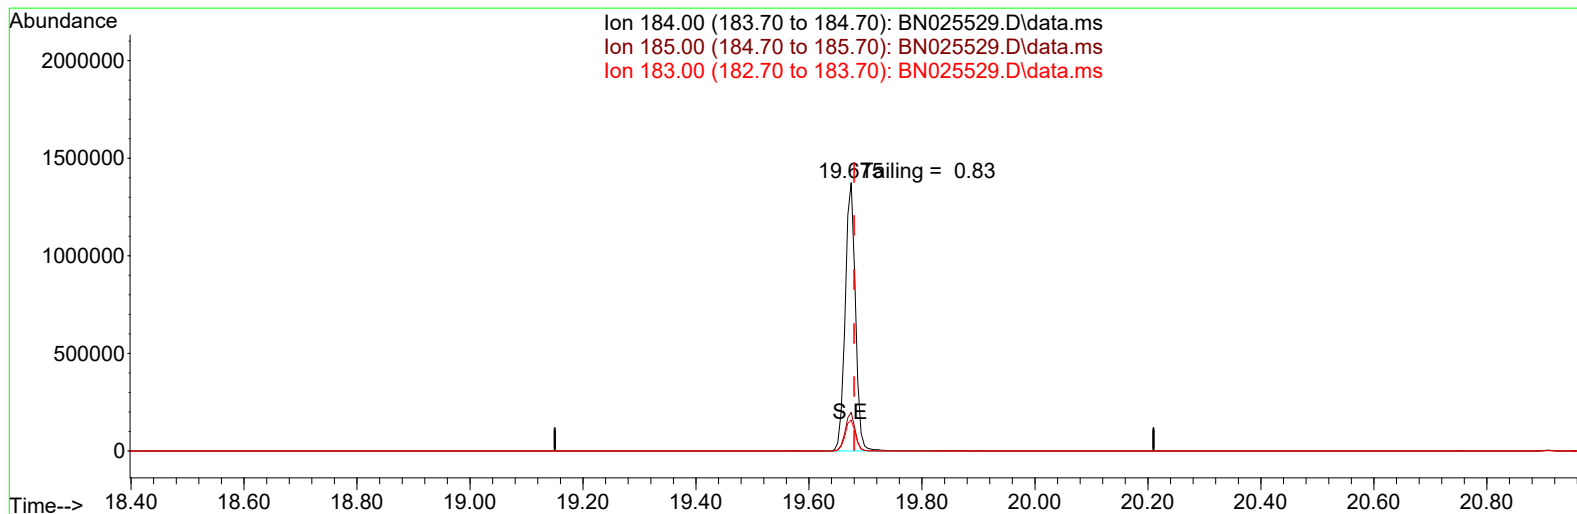

TIC: BN025529.D\data.ms

(77) Benzidine

19.675min (-0.006) 0.00 ng

response 1728066

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.39
183.00	13.20	11.57
0.00	0.00	0.00