


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN052021\
Data File : BN014683.D
Acq On : 20 May 2021 16:47
Operator : CG/JU
Sample : M2465-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YARK0

Manual Integrations
APPROVED

mohammad
5/21/2021 3:22:20 PM

Quant Time: May 20 17:21:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 20 16:48:16 2021
Response via : Initial Calibration

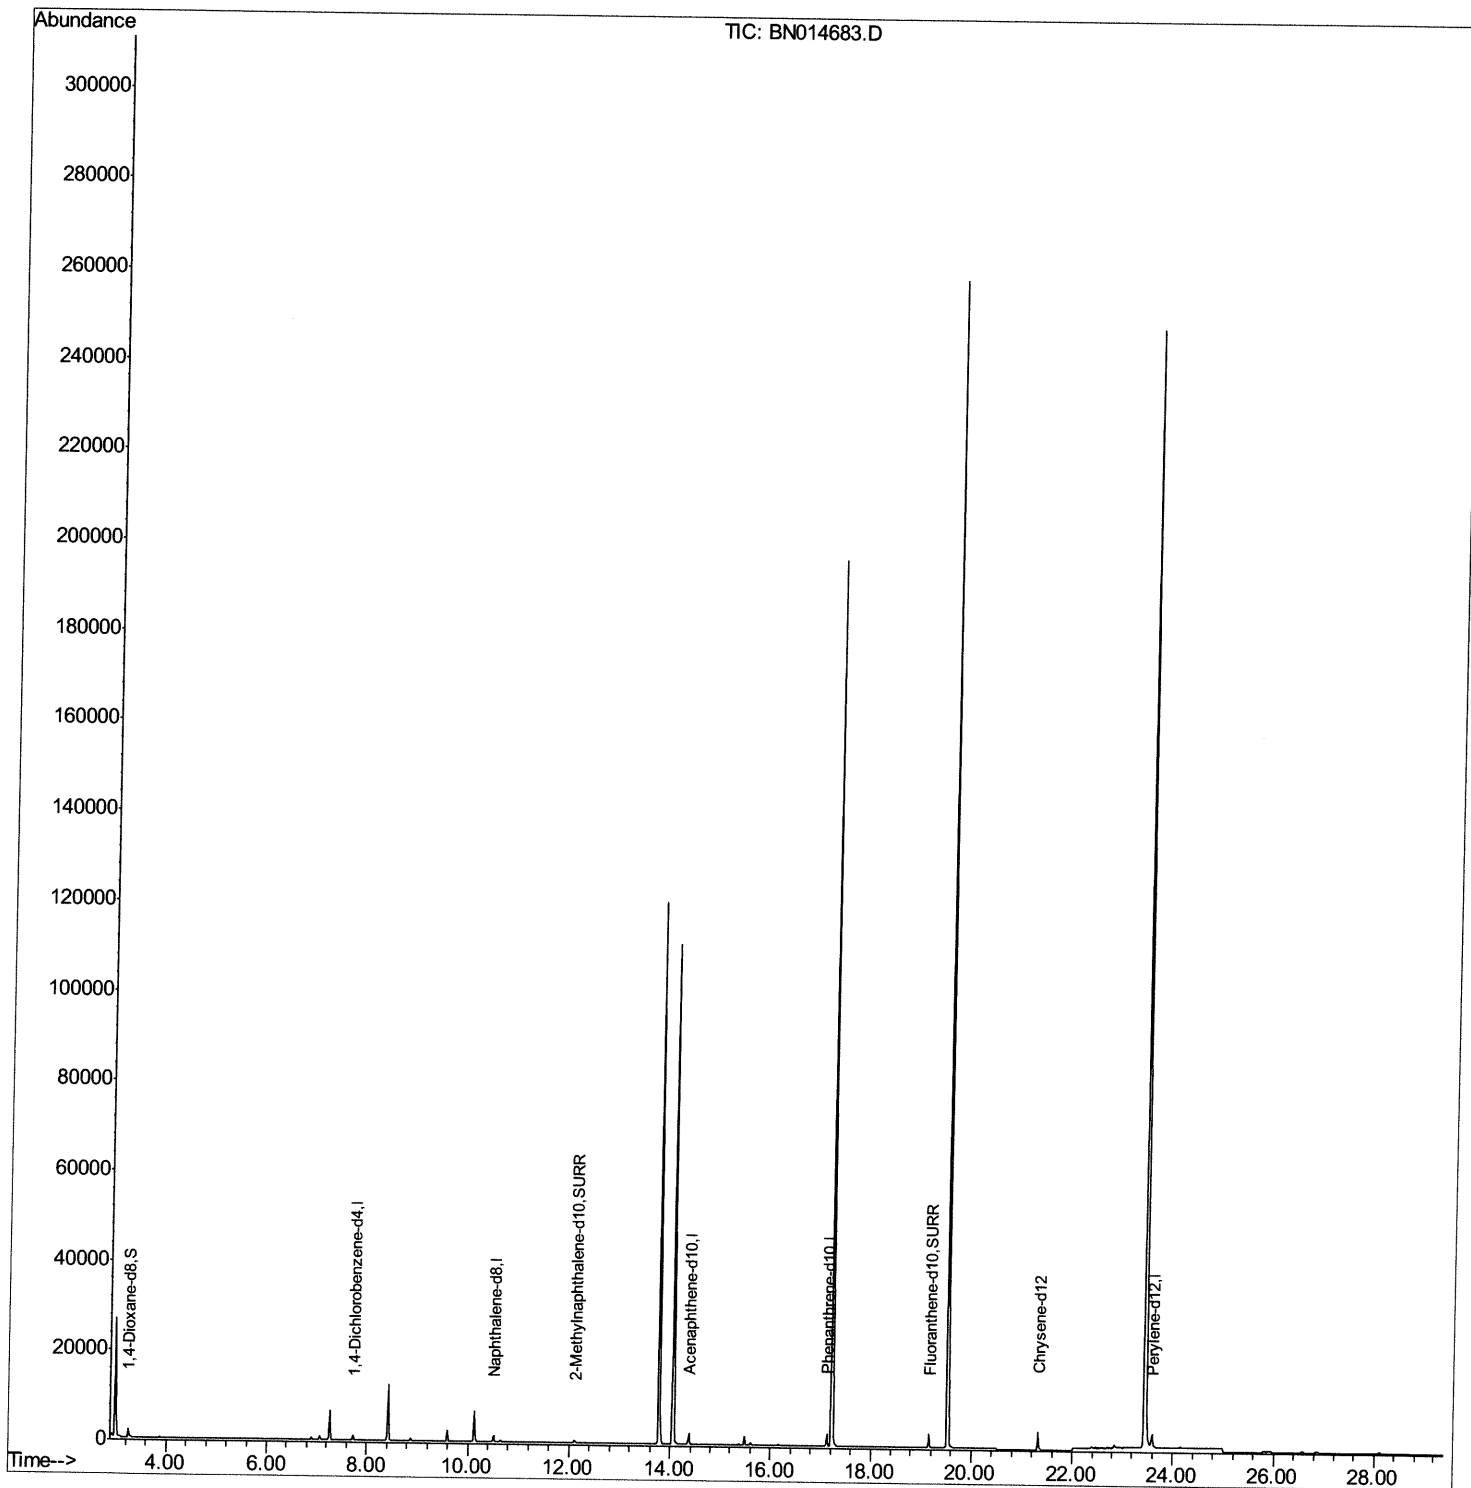

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN052021\
 Data File : BN014683.D
 Acq On : 20 May 2021 16:47
 Operator : CG/JU
 Sample : M2465-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YARKO

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:22:20 PM

Quant Time: May 20 17:19:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 20 16:48:16 2021
 Response via : Initial Calibration

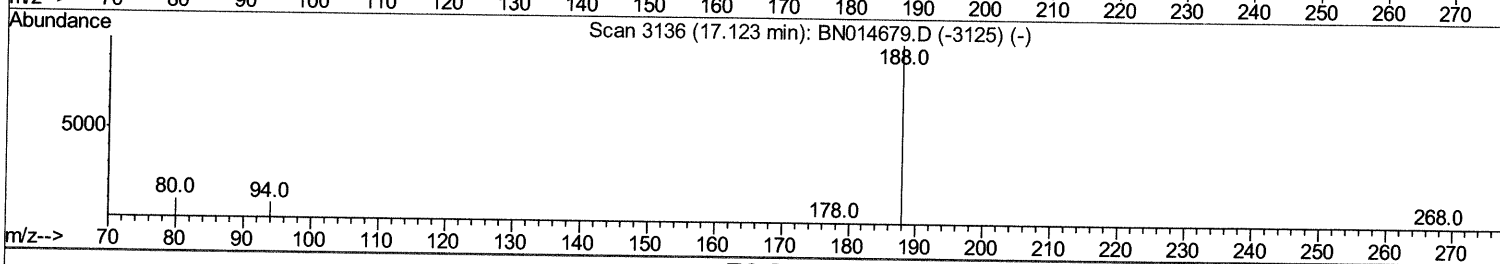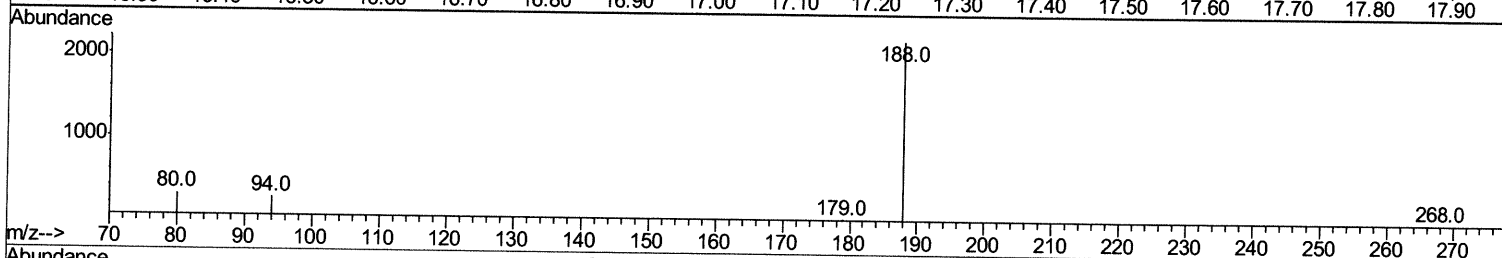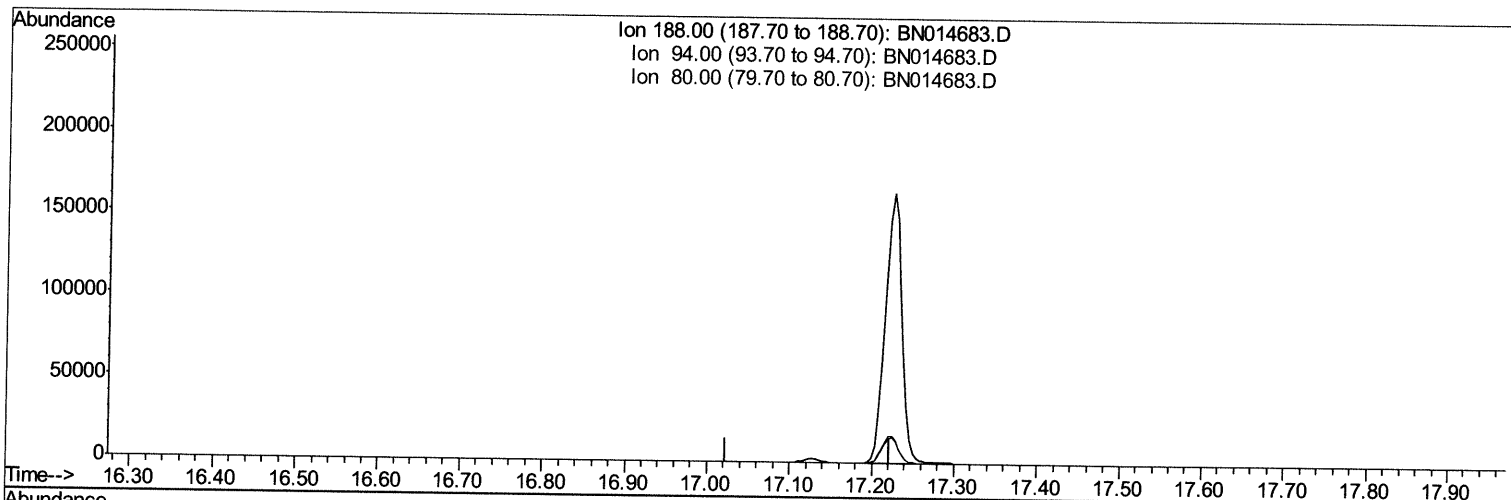

TIC: BN014683.D

(13) Phenanthrene-d10 (I)

17.123min (-17.123) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.10	0.00#
80.00	12.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN052021\
 Data File : BN014683.D
 Acq On : 20 May 2021 16:47
 Operator : CG/JU
 Sample : M2465-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 YARK0

Manual Integrations
APPROVED

mohammad
 5/21/2021 3:22:20 PM

Quant Time: May 20 17:19:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 20 16:48:16 2021
 Response via : Initial Calibration

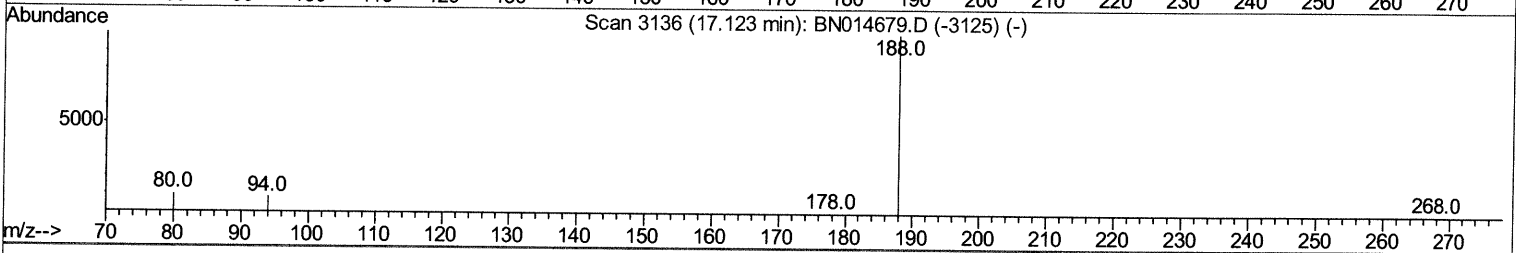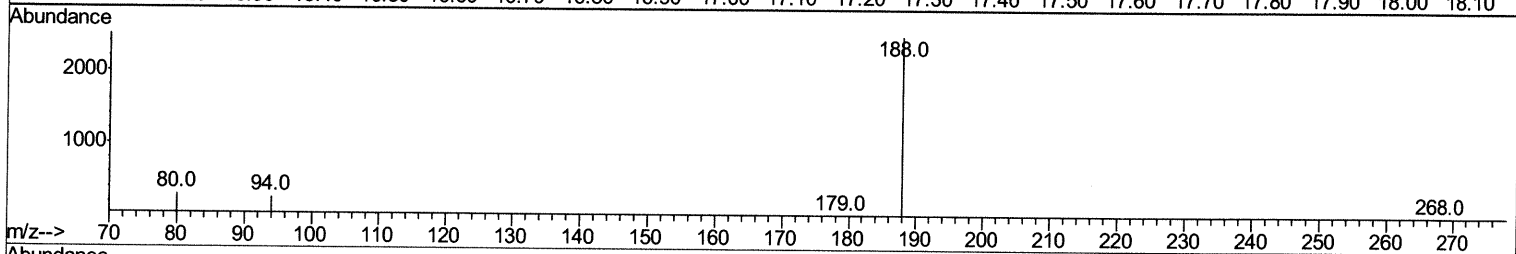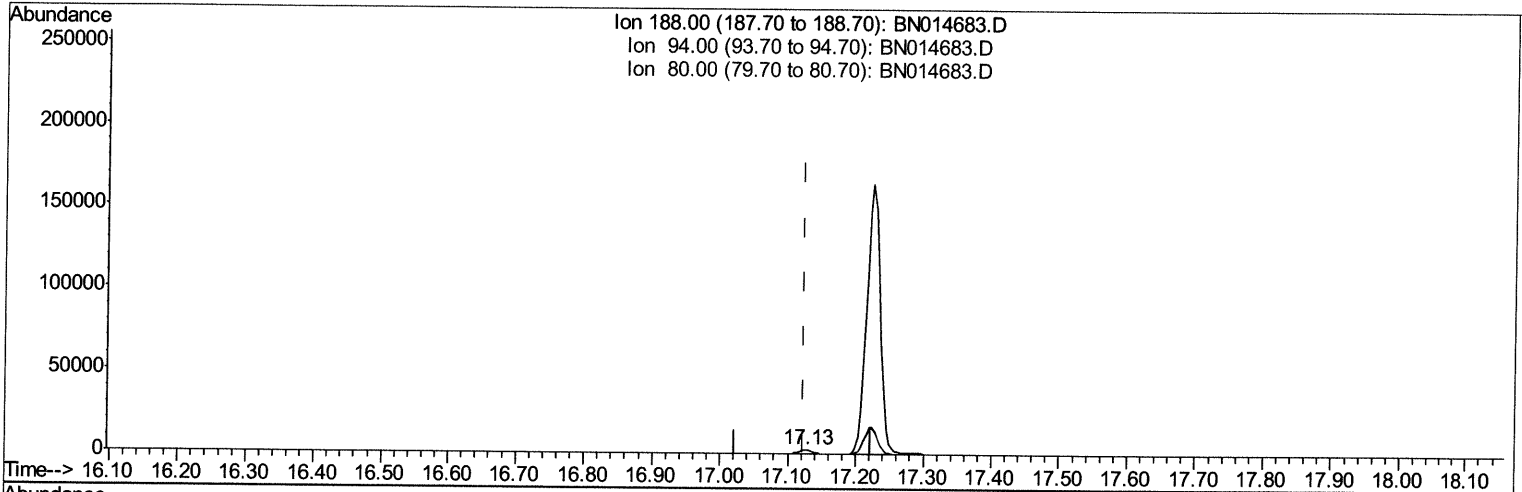

TIC: BN014683.D

(13) Phenanthrene-d10 (I)

17.127min (+0.004) 0.40ng/ul m 05/25/21JU

response 3359

Ion	Exp%	Act%
188.00	100	100
94.00	11.10	10.93
80.00	12.50	11.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN052021\
Data File : BN014683.D
Acq On : 20 May 2021 16:47
Operator : CG/JU
Sample : M2465-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YARK0

Manual Integrations
APPROVED

mohammad
5/21/2021 3:22:20 PM

Quant Time: May 20 17:21:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 20 16:48:16 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	535	0.40	ng/ul	0.00
4) Naphthalene-d8	10.51	136	1809	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.38	164	1380	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.13	188	3359m >	0.40	ng/ul >	0.00
17) Chrysene-d12	21.32	240	3783	0.40	ng/ul	0.00
23) Perylene-d12	23.59	264	3788	0.40	ng/ul	0.00

05/23/21 JU

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	1395	2.54	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.11	152	881	0.28	ng/ul	0.00
18) Fluoranthene-d10	19.16	212	3544	0.37	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed